

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Alamance Instrument Location Bar Mobility
Instrument Serial No. 008615 Burlington PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jonya B Skinnin
Signature of Certifying Official

644
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE CO BAT MOBILE UNIT 4 001

Serial Number: 008615
Test Date: 03/14/2019

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Female

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: SKINNER, TONYA B

Permit Number: 13651E

Effective:

08/01/2017-08/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG716201

Exp Date: 06/11/2019

Test	g/210L	Time
DIAG	Pass	10:12pm
AIR BLK	.00	10:13pm
ACCY CHK	.07	10:14pm
AIR BLK	.00	10:14pm
SUB TEST	.00	10:15pm
AIR BLK	.00	10:16pm
SUB TEST	.00	10:17pm
AIR BLK	.00	10:18pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ALAMANCE CO BAT MOBILE UNIT 4 001

Serial Number: 008615 Test Record Number: 5581
Test Date: 03/14/2019 Test Time: 10:19pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:20pm
FLO	Pass	10:20pm
FC	Pass	10:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:20pm
SRC	Pass	10:20pm
DET	Pass	10:20pm
BAR	Pass	10:20pm
BT	Pass	10:20pm

Blank Tests

Test	Status	Time
AIR	Pass	10:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:21pm

CRC Tests

Test	Status	Time
COMP	Pass	10:21pm
CAL	Pass	10:21pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Alleghany Instrument Location Alleghany County
Instrument Serial No. 008890 Jail
Sparta, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Dale Farley
Signature of Certifying Official

655
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALLEGHANY COUNTY ALLEGHANY CO JAIL 020

Serial Number: 008890
Test Date: 03/19/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Female
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: FARLEY, CYNTHIA D
Permit Number: 24123E
Effective:
11/01/2018-11/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG821801
Exp Date: 08/06/2020

Test	g/210L	Time
DIAG	Pass	2:08pm
AIR BLK	.00	2:08pm
ACCY CHK	.07	2:09pm
AIR BLK	.00	2:10pm
SUB TEST	.00	2:11pm
AIR BLK	.00	2:11pm
SUB TEST	.00	2:13pm
AIR BLK	.00	2:14pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

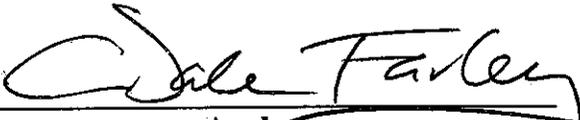
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ALLEGHANY COUNTY ALLEGHANY CO JAIL 020

Serial Number: 008890 Test Record Number: 756
Test Date: 03/19/2019 Test Time: 2:15pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:15pm
FLO	Pass	2:15pm
FC	Pass	2:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:15pm
SRC	Pass	2:15pm
DET	Pass	2:15pm
BAR	Pass	2:15pm
BT	Pass	2:15pm

Blank Tests

Test	Status	Time
AIR	Pass	2:16pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:16pm

CRC Tests

Test	Status	Time
COMP	Pass	2:16pm
CAL	Pass	2:16pm

Preventive Maintenance
Status: Pass

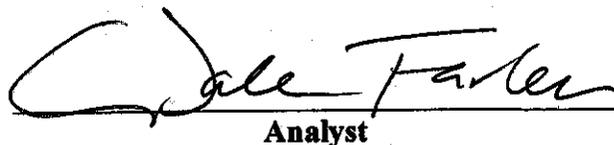
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County ANSON Instrument Location ANSON COUNTY

Instrument Serial No. 008597 SHERIFF'S OFFICE
WADESBORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of MARCH, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan F. Barnes
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ANSON COUNTY SHERIFF'S OFFICE 030

Serial Number: 008597
Test Date: 03/20/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 15671E
Effective:
07/01/2017-07/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG902202
Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	1:13pm
AIR BLK	.00	1:14pm
ACCY CHK	.08	1:15pm
AIR BLK	.00	1:16pm
SUB TEST	.00	1:16pm
AIR BLK	.00	1:17pm
SUB TEST	.00	1:19pm
AIR BLK	.00	1:20pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ANSON COUNTY SHERIFF'S OFFICE 030

Serial Number: 008597 Test Record Number: 1720
Test Date: 03/20/2019 Test Time: 1:20pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:21pm
FLO	Pass	1:21pm
FC	Pass	1:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:21pm
SRC	Pass	1:21pm
DET	Pass	1:21pm
BAR	Pass	1:21pm
BT	Pass	1:21pm

Blank Tests

Test	Status	Time
AIR	Pass	1:21pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:21pm

CRC Tests

Test	Status	Time
COMP	Pass	1:22pm
CAL	Pass	1:22pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County ANSON Instrument Location ANSON COUNTY
Instrument Serial No. 008739 SHERIFF'S OFFICE
WADES BORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of MARCH, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Benson
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ANSON COUNTY SHERIFF'S OFFICE 030

Serial Number: 008739
Test Date: 03/20/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 15671E

Effective:

07/01/2017-07/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG902202


Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	1:09pm
AIR BLK	.00	1:10pm
ACCY CHK	.08	1:10pm
AIR BLK	.00	1:12pm
SUB TEST	.00	1:12pm
AIR BLK	.00	1:13pm
SUB TEST	.00	1:15pm
AIR BLK	.00	1:15pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ANSON COUNTY SHERIFF'S OFFICE 030

Serial Number: 008739 Test Record Number: 381
Test Date: 03/20/2019 Test Time: 1:16pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:16pm
FLO	Pass	1:16pm
FC	Pass	1:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:17pm
SRC	Pass	1:17pm
DET	Pass	1:17pm
BAR	Pass	1:17pm
BT	Pass	1:17pm

Blank Tests

Test	Status	Time
AIR	Pass	1:17pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:17pm

CRC Tests

Test	Status	Time
COMP	Pass	1:17pm
CAL	Pass	1:17pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Ashe Instrument Location Ashe County
Instrument Serial No. 008849 Gail
Jefferson, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of March, 20 19, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Dale Farley
Signature of Certifying Official

655
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ASHE COUNTY ASHE COUNTY JAIL 040

Serial Number: 008849
Test Date: 03/19/2019

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Female

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: FARLEY, CYNTHIA D

Permit Number: 24123E

Effective:

11/01/2018-11/01/2020

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG805801


Exp Date: 02/27/2020

Test	g/210L	Time
DIAG	Pass	4:21pm
AIR BLK	.00	4:22pm
ACCY CHK	.07	4:22pm
AIR BLK	.00	4:24pm
SUB TEST	.00	4:24pm
AIR BLK	.00	4:25pm
SUB TEST	.00	4:27pm
AIR BLK	.00	4:28pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

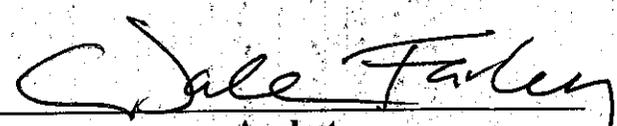

Analyst

Intox EC/IR-II: Preventive Maintenance

ASHE COUNTY ASHE COUNTY JAIL 040

Serial Number: 008849 Test Record Number: 1227
Test Date: 03/19/2019 Test Time: 4:29pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	4:29pm
FLO	Pass	4:29pm
FC	Pass	4:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:29pm
SRC	Pass	4:29pm
DET	Pass	4:29pm
BAR	Pass	4:29pm
BT	Pass	4:29pm

Blank Tests

Test	Status	Time
AIR	Pass	4:30pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:30pm

CRC Tests

Test	Status	Time
COMP	Pass	4:30pm
CAL	Pass	4:30pm

Preventive Maintenance
Status: Pass

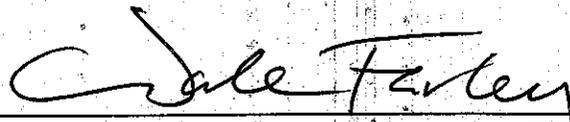

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Avery Instrument Location Banner Elk PD
Instrument Serial No. 008724 Banner Elk, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

AVERY COUNTY BANNER ELK PD 050

Serial Number: 008724

Test Date: 03/20/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J

Permit Number: 11304E

Effective:

05/01/2017-05/01/2019

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG716202

Exp Date: 06/11/2019

Test	g/210L	Time
DIAG	Pass	2:12pm
AIR BLK	.00	2:13pm
ACCY CHK	.07	2:14pm
AIR BLK	.00	2:15pm
SUB TEST	.00	2:15pm
AIR BLK	.00	2:16pm
SUB TEST	.00	2:18pm
AIR BLK	.00	2:19pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

AVERY COUNTY BANNER ELK PD 050

Serial Number: 008724 Test Record Number: 579
Test Date: 03/20/2019 Test Time: 2:20pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:20pm
FLO	Pass	2:20pm
FC	Pass	2:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:20pm
SRC	Pass	2:20pm
DET	Pass	2:20pm
BAR	Pass	2:20pm
BT	Pass	2:20pm

Blank Tests

Test	Status	Time
AIR	Pass	2:21pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:21pm

CRC Tests

Test	Status	Time
COMP	Pass	2:21pm
CAL	Pass	2:21pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Beaufort Instrument Location Beaufort Co. Courthouse
Instrument Serial No. 008586 102 E. 2nd St., Washington, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of MARCH, 20 19 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Lincoln Keel
Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BEAUFORT COUNTY COURTHOUSE 060

Serial Number: 008586
Test Date: 03/19/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: KEESLER, LINDA A
Permit Number: 11646E
Effective:
08/01/2017-08/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG821801
Exp Date: 08/06/2020


Test	g/210L	Time
DIAG	Pass	11:29am
AIR BLK	.00	11:30am
ACCY CHK	.08	11:30am
AIR BLK	.00	11:32am
SUB TEST	.00	11:32am
AIR BLK	.00	11:33am
SUB TEST	.00	11:35am
AIR BLK	.00	11:35am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

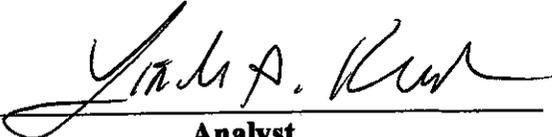

Analyst

Intox EC/IR-II: Preventive Maintenance

BEAUFORT COUNTY COURTHOUSE 060

Serial Number: 008586 Test Record Number: 1461
Test Date: 03/19/2019 Test Time: 11:38am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:39am
FLO	Pass	11:39am
FC	Pass	11:39am

Temperature Tests

Test	Status	Time
FC1	Pass	11:39am
SRC	Pass	11:39am
DET	Pass	11:39am
BAR	Pass	11:39am
BT	Pass	11:39am

Blank Tests

Test	Status	Time
AIR	Pass	11:39am


Printer Tests

Test	Status	Time
PRNT	Pass	11:39am

CRC Tests

Test	Status	Time
COMP	Pass	11:40am
CAL	Pass	11:40am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Beaufort Instrument Location Beaufort Co. Courthouse
Instrument Serial No. 008909 102 E. 2nd St., Washington, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of MARCH, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Linnea Keene
Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BEAUFORT COUNTY COURTHOUSE 060

Serial Number: 008909
Test Date: 03/19/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: KEESLER, LINDA A
Permit Number: 11646E
Effective:
08/01/2017-08/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG821801
Exp Date: 08/06/2020


Test	g/210L	Time
DIAG	Pass	11:30am
AIR BLK	.00	11:32am
ACCY CHK	.08	11:32am
AIR BLK	.00	11:33am
SUB TEST	.00	11:34am
AIR BLK	.00	11:35am
SUB TEST	.00	11:37am
AIR BLK	.00	11:38am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BEAUFORT COUNTY COURTHOUSE 060

Serial Number: 008909 Test Record Number: 3249
Test Date: 03/19/2019 Test Time: 11:39am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:39am
FLO	Pass	11:39am
FC	Pass	11:39am

Temperature Tests

Test	Status	Time
FC1	Pass	11:39am
SRC	Pass	11:39am
DET	Pass	11:39am
BAR	Pass	11:39am
BT	Pass	11:39am

Blank Tests

Test	Status	Time
AIR	Pass	11:40am


Printer Tests

Test	Status	Time
PRNT	Pass	11:40am

CRC Tests

Test	Status	Time
COMP	Pass	11:40am
CAL	Pass	11:40am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Bertie Instrument Location Bertie C.S.O.
Instrument Serial No. 008897 222 County Farm Rd., Windsor, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BERTIE COUNTY BERTIE CO SO 070

Serial Number: 008897
Test Date: 03/28/2019

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GUARD, KELLY G

Permit Number: 12955E

Effective:

06/01/2017-06/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG721401

Exp Date: 08/02/2019

Test	g/210L	Time
DIAG	Pass	11:08am
AIR BLK	.00	11:09am
ACCY CHK	.07	11:10am
AIR BLK	.00	11:11am
SUB TEST	.00	11:12am
AIR BLK	.00	11:13am
SUB TEST	.00	11:15am
AIR BLK	.00	11:16am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

BERTIE COUNTY BERTIE CO SO 070

Serial Number: 008897 Test Record Number: 1199
Test Date: 03/28/2019 Test Time: 11:17am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:17am
FLO	Pass	11:17am
FC	Pass	11:17am

Temperature Tests

Test	Status	Time
FC1	Pass	11:17am
SRC	Pass	11:17am
DET	Pass	11:17am
BAR	Pass	11:17am
BT	Pass	11:17am

Blank Tests

Test	Status	Time
AIR	Pass	11:18am

Printer Tests

Test	Status	Time
PRNT	Pass	11:18am

CRC Tests

Test	Status	Time
COMP	Pass	11:18am
CAL	Pass	11:18am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Brunswick Instrument Location BAT Mobile Unit #5

Instrument Serial No. 8826 Culabash, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY BAT MOBILE UNIT 5 090

Serial Number: 008826
Test Date: 03/29/2019

Citation Number: M0000000-0
Subject's Name: NONE, NONE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: TODD, SHANE C
Permit Number: 11391E
Effective:
07/27/2018-07/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG807101
Exp Date: 03/12/2020

Test	g/210L	Time
DIAG	Pass	11:29pm
AIR BLK	.00	11:30pm
ACCY CHK	.08	11:31pm
AIR BLK	.00	11:32pm
SUB TEST	.00	11:33pm
AIR BLK	.00	11:34pm
SUB TEST	.00	11:35pm
AIR BLK	.00	11:36pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY BAT MOBILE UNIT 5 090

Serial Number: 008826 Test Record Number: 8097
Test Date: 03/29/2019 Test Time: 11:46pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:47pm
FLO	Pass	11:47pm
FC	Pass	11:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:47pm
SRC	Pass	11:47pm
DET	Pass	11:47pm
BAR	Pass	11:47pm
BT	Pass	11:47pm

Blank Tests

Test	Status	Time
AIR	Pass	11:48pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:48pm

CRC Tests

Test	Status	Time
COMP	Pass	11:48pm
CAL	Pass	11:48pm

Preventive Maintenance
Status: Pass

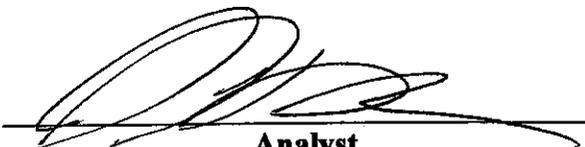
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Brunswick Instrument Location BAT Mobile Unit #5
Instrument Serial No. 8704 Calabash, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of March, 20 19, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY BAT MOBILE UNIT 5 090

Serial Number: 008704 Test Record Number: 541
Test Date: 03/29/2019 Test Time: 11:34pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:34pm
FLO	Pass	11:34pm
FC	Pass	11:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:35pm
SRC	Pass	11:35pm
DET	Pass	11:35pm
BAR	Pass	11:35pm
BT	Pass	11:35pm

Blank Tests

Test	Status	Time
AIR	Pass	11:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:35pm

CRC Tests

Test	Status	Time
COMP	Pass	11:35pm
CAL	Pass	11:35pm

Preventive Maintenance
Status: Pass


Analyst

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY BAT MOBILE UNIT 5 090

Serial Number: 008704 Test Record Number: 541
Test Date: 03/29/2019 Test Time: 11:34pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:34pm
FLO	Pass	11:34pm
FC	Pass	11:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:35pm
SRC	Pass	11:35pm
DET	Pass	11:35pm
BAR	Pass	11:35pm
BT	Pass	11:35pm

Blank Tests

Test	Status	Time
AIR	Pass	11:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:35pm

CRC Tests

Test	Status	Time
COMP	Pass	11:35pm
CAL	Pass	11:35pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Cabarrus Instrument Location Kannapolis PD
Instrument Serial No. 008589 401 Louette Way Kannapolis

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of March, 20 19, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Mark D. [Signature]
Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY KANNAPOLIS PD 120

Serial Number: 008589
Test Date: 03/25/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HAYS, MARK D

Permit Number: 15924E

Effective:

01/01/2018-01/01/2020

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG814902

Exp Date: 05/29/2020


Test	g/210L	Time
DIAG	Pass	11:28am
AIR BLK	.00	11:29am
ACCY CHK	.08	11:29am
AIR BLK	.00	11:30am
SUB TEST	.00	11:31am
AIR BLK	.00	11:32am
SUB TEST	.00	11:33am
AIR BLK	.00	11:35am

Reported AC: .00 g/210L

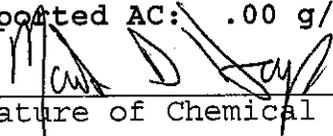

Signature of Chemical Analyst

Court CVR

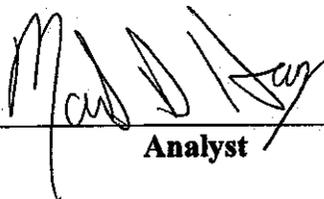

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY KANNAPOLIS PD 120

Serial Number: 008589 Test Record Number: 2965
Test Date: 03/25/2019 Test Time: 11:36am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:37am
FLO	Pass	11:37am
FC	Pass	11:37am

Temperature Tests

Test	Status	Time
FC1	Pass	11:37am
SRC	Pass	11:37am
DET	Pass	11:37am
BAR	Pass	11:37am
BT	Pass	11:37am

Blank Tests

Test	Status	Time
AIR	Pass	11:38am

Printer Tests

Test	Status	Time
PRNT	Pass	11:38am

CRC Tests

Test	Status	Time
COMP	Pass	11:38am
CAL	Pass	11:38am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Caldwell Instrument Location Caldwell Co. Jail

Instrument Serial No. 008719 Leasick, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY CALDWELL COUNTY JAIL
130

Serial Number: 008719
Test Date: 03/22/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J

Permit Number: 11304E

Effective:

05/01/2017-05/01/2019

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG814901

Exp Date: 05/29/2020

Test	g/210L	Time
DIAG	Pass	3:30pm
AIR BLK	.00	3:31pm
ACCY CHK	.07	3:31pm
AIR BLK	.00	3:32pm
SUB TEST	.00	3:33pm
AIR BLK	.00	3:34pm
SUB TEST	.00	3:36pm
AIR BLK	.00	3:37pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY CALDWELL COUNTY JAIL 130

Serial Number: 008719 Test Record Number: 2459
Test Date: 03/22/2019 Test Time: 3:44pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:45pm
FLO	Pass	3:45pm
FC	Pass	3:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:45pm
SRC	Pass	3:45pm
DET	Pass	3:45pm
BAR	Pass	3:45pm
BT	Pass	3:45pm

Blank Tests

Test	Status	Time
AIR	Pass	3:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:46pm

CRC Tests

Test	Status	Time
COMP	Pass	3:46pm
CAL	Pass	3:46pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Caldwell Instrument Location Caldwell Co Jail

Instrument Serial No. 008803 Kenoin, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

049
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY CALDWELL COUNTY JAIL
130

Serial Number: 008803
Test Date: 03/22/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J

Permit Number: 11304E

Effective:

05/01/2017-05/01/2019

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG902201


Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	3:29pm
AIR BLK	.00	3:30pm
ACCY CHK	.07	3:31pm
AIR BLK	.00	3:32pm
SUB TEST	.00	3:32pm
AIR BLK	.00	3:33pm
SUB TEST	.00	3:35pm
AIR BLK	.00	3:36pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY CALDWELL COUNTY JAIL 130

Serial Number: 008803 Test Record Number: 562
Test Date: 03/22/2019 Test Time: 3:37pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:37pm
FLO	Pass	3:37pm
FC	Pass	3:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:38pm
SRC	Pass	3:38pm
DET	Pass	3:38pm
BAR	Pass	3:38pm
BT	Pass	3:38pm

Blank Tests

Test	Status	Time
AIR	Pass	3:38pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:38pm

CRC Tests

Test	Status	Time
COMP	Pass	3:38pm
CAL	Pass	3:38pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County CASWELL Instrument Location CASWELL CO. DETENTION CENTER

Instrument Serial No. 008593 211 COUNTY PARK RD YANCEYVILLE, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of MARCH, 20 19 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



B. D. Smith
Signature of Certifying Official

637
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CASWELL COUNTY DETENTION CENTER 160

Serial Number: 008593
Test Date: 03/11/2019

Citation Number: M0000000-0
Subject's Name:

~~PREVENTIVE, MAINTENANCE~~

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: SMITH, BRIAN D

Permit Number: 08937E

Effective:

08/01/2017-08/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG734101

Exp Date: 12/07/2019


Test	g/210L	Time
DIAG	Pass	3:40pm
AIR BLK	.00	3:41pm
ACCY CHK	.07	3:42pm
AIR BLK	.00	3:43pm
SUB TEST	.00	3:43pm
AIR BLK	.00	3:44pm
SUB TEST	.00	3:46pm
AIR BLK	.00	3:47pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CASWELL COUNTY DETENTION CENTER 160

Serial Number: 008593 Test Record Number: 1659
Test Date: 03/11/2019 Test Time: 3:47pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	3:48pm
FLO	Pass	3:48pm
FC	Pass	3:48pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:48pm
SRC	Pass	3:48pm
DET	Pass	3:48pm
BAR	Pass	3:48pm
BT	Pass	3:48pm

Blank Tests

Test	Status	Time
AIR	Pass	3:49pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:49pm

CRC Tests

Test	Status	Time
COMP	Pass	3:49pm
CAL	Pass	3:49pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Catawba

Instrument Location Catawba County SO


Instrument Serial No. 008821

100 B Southwest Blvd, Newton

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7th day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hill
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY CATAWBA COUNTY SD 170

Serial Number: 008821
Test Date: 03/07/2019

Citation Number: M0000000-0
Subject's Name:

~~PREVENTIVE, MAINTENANCE~~

Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: HUTCHINSON, JOSEPH E
Permit Number: 19951E
Effective:
08/01/2017-08/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG814901
Exp Date: 05/29/2020


Test	g/210L	Time
DIAG	Pass	5:15pm
AIR BLK	.00	5:16pm
ACCY CHK	.07	5:17pm
AIR BLK	.00	5:17pm
SUB TEST	.00	5:18pm
AIR BLK	.00	5:19pm
SUB TEST	.00	5:20pm
AIR BLK	.00	5:22pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

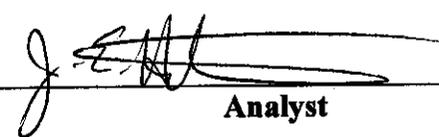

Analyst

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY CATAWBA COUNTY SD 170

Serial Number: 008821 Test Record Number: 1992
Test Date: 03/07/2019 Test Time: 5:24pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:24pm
FLO	Pass	5:24pm
FC	Pass	5:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:24pm
SRC	Pass	5:24pm
DET	Pass	5:24pm
BAR	Pass	5:24pm
BT	Pass	5:24pm

Blank Tests

Test	Status	Time
AIR	Pass	5:25pm


Printer Tests

Test	Status	Time
PRNT	Pass	5:25pm

CRC Tests

Test	Status	Time
COMP	Pass	5:25pm
CAL	Pass	5:25pm

Preventive Maintenance
Status: Pass

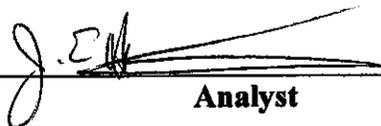

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Catawba Instrument Location Hickory PD
Instrument Serial No. 008841 347 2nd Ave. SW, Hickory

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY HICKORY PD 170

Serial Number: 008841
Test Date: 03/21/2019

Citation Number: M0000000-0
Subject's Name:

~~PREVENTIVE, MAINTENANCE~~

Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: HAYS, MARK D
Permit Number: 15924E
Effective:
01/01/2018-01/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG821801
Exp Date: 08/06/2020


Test	g/210L	Time
DIAG	Pass	8:54am
AIR BLK	.00	8:55am
ACCY CHK	.08	8:56am
AIR BLK	.00	8:57am
SUB TEST	.00	8:58am
AIR BLK	.00	8:59am
SUB TEST	.00	9:00am
AIR BLK	.00	9:01am

Reported AC: .00 g/210L

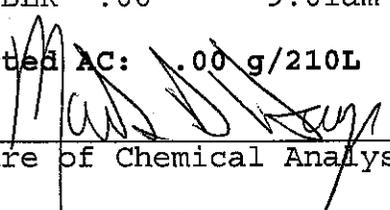

Signature of Chemical Analyst

Court CVR

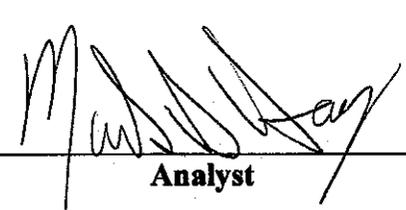

Analyst

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY HICKORY PD 170

Serial Number: 008841 Test Record Number: 1908
Test Date: 03/21/2019 Test Time: 9:05am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:05am
FLO	Pass	9:05am
FC	Pass	9:05am

Temperature Tests

Test	Status	Time
FC1	Pass	9:05am
SRC	Pass	9:05am
DET	Pass	9:05am
BAR	Pass	9:05am
BT	Pass	9:05am

Blank Tests

Test	Status	Time
AIR	Pass	9:06am

Printer Tests

Test	Status	Time
PRNT	Pass	9:06am

CRC Tests

Test	Status	Time
COMP	Pass	9:06am
CAL	Pass	9:06am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II


County Catawba Instrument Location Catawba County SO

Instrument Serial No. 008687 100 B SW Blvd., Newton

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of March, 20 19, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY CATAWBA COUNTY SD 170

Serial Number: 008687
Test Date: 03/25/2019

Citation Number: M0000000-0
Subject's Name:

~~PREVENTIVE, MAINTENANCE~~

Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: HAYS, MARK D
Permit Number: 15924E
Effective:
01/01/2018-01/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG821401
Exp Date: 08/02/2020


Test	g/210L	Time
DIAG	Pass	9:35am
AIR BLK	.00	9:36am
ACCY. CHK	.07	9:37am
AIR BLK	.00	9:38am
SUB TEST	.00	9:39am
AIR BLK	.00	9:40am
SUB TEST	.00	9:42am
AIR BLK	.00	9:42am

Reported AC: .00 g/210L

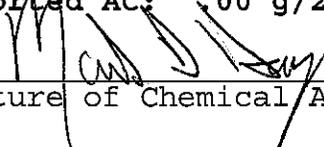

Signature of Chemical Analyst

Court CVR

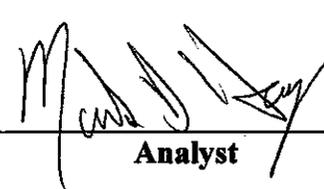

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY CATAWBA COUNTY SD 170

Serial Number: 008687 Test Record Number: 2797
Test Date: 03/25/2019 Test Time: 9:44am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:44am
FLO	Pass	9:44am
FC	Pass	9:44am

Temperature Tests

Test	Status	Time
FC1	Pass	9:45am
SRC	Pass	9:45am
DET	Pass	9:45am
BAR	Pass	9:45am
BT	Pass	9:45am

Blank Tests

Test	Status	Time
AIR	Pass	9:45am

Printer Tests

Test	Status	Time
PRNT	Pass	9:45am

CRC Tests

Test	Status	Time
COMP	Pass	9:45am
CAL	Pass	9:45am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Cherokee Instrument Location Cherokee Co. Jail

Instrument Serial No. 008622 Murphy, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of March, 20 19 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



David R. Cuthbert
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHEROKEE COUNTY CHEROKEE COUNTY JAIL
190

Serial Number: 008622
Test Date: 03/28/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: CUTLER, DANIEL R

Permit Number: 08457E

Effective:

09/01/2017-09/01/2019

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG734102

Exp Date: 12/07/2019

Test	g/210L	Time
DIAG	Pass	9:07am
AIR BLK	.00	9:08am
ACCY CHK	.07	9:08am
AIR BLK	.00	9:09am
SUB TEST	.00	9:10am
AIR BLK	.00	9:11am
SUB TEST	.00	9:13am
AIR BLK	.00	9:14am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CHEROKEE COUNTY CHEROKEE COUNTY JAIL 190

Serial Number: 008622 Test Record Number: 1080
Test Date: 03/28/2019 Test Time: 9:21am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:22am
FLO	Pass	9:22am
FC	Pass	9:22am

Temperature Tests

Test	Status	Time
FC1	Pass	9:22am
SRC	Pass	9:22am
DET	Pass	9:22am
BAR	Pass	9:22am
BT	Pass	9:22am

Blank Tests

Test	Status	Time
AIR	Pass	9:23am


Printer Tests

Test	Status	Time
PRNT	Pass	9:23am

CRC Tests

Test	Status	Time
COMP	Pass	9:23am
CAL	Pass	9:23am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Cherokee Instrument Location Cherokee Co. Jail

Instrument Serial No. 008711 Murphy, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul R. Luthin
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHEROKEE COUNTY CHEROKEE COUNTY JAIL
190

Serial Number: 008711
Test Date: 03/28/2019

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: CUTLER, DANIEL R
Permit Number: 08457E
Effective:
09/01/2017-09/01/2019

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG716202
Exp Date: 06/11/2019

Test	g/210L	Time
DIAG	Pass	9:07am
AIR BLK	.00	9:08am
ACCY CHK	.07	9:09am
AIR BLK	.00	9:10am
SUB TEST	.00	9:11am
AIR BLK	.00	9:12am
SUB TEST	.00	9:13am
AIR BLK	.00	9:14am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CHEROKEE COUNTY CHEROKEE COUNTY JAIL 190

Serial Number: 008711 Test Record Number: 977
Test Date: 03/28/2019 Test Time: 9:15am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:15am
FLO	Pass	9:15am
FC	Pass	9:16am

Temperature Tests

Test	Status	Time
FC1	Pass	9:16am
SRC	Pass	9:16am
DET	Pass	9:16am
BAR	Pass	9:16am
BT	Pass	9:16am

Blank Tests

Test	Status	Time
AIR	Pass	9:16am


Printer Tests

Test	Status	Time
PRNT	Pass	9:16am

CRC Tests

Test	Status	Time
COMP	Pass	9:17am
CAL	Pass	9:17am

Preventive Maintenance
Status: Pass

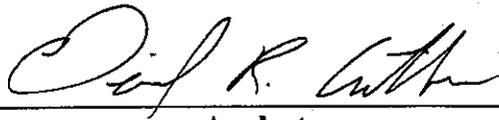

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Chowan Instrument Location Chowan Co. Public Safety

Instrument Serial No. 008895 Center, 305 Freemason St., Edenboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHOWAN COUNTY PUBLIC SAFETY CENTER 200

Serial Number: 008895

Test Date: 03/28/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GUARD, KELLY G

Permit Number: 12955E

Effective:

06/01/2017-06/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG902201

Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	9:59am
AIR BLK	.00	10:00am
ACCY CHK	.08	10:00am
AIR BLK	.00	10:02am
SUB TEST	.00	10:02am
AIR BLK	.00	10:03am
SUB TEST	.00	10:05am
AIR BLK	.00	10:06am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CHOWAN COUNTY PUBLIC SAFETY CENTER 200

Serial Number: 008895 Test Record Number: 886
Test Date: 03/28/2019 Test Time: 10:11am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:11am
FLO	Pass	10:11am
FC	Pass	10:11am

Temperature Tests

Test	Status	Time
FC1	Pass	10:11am
SRC	Pass	10:11am
DET	Pass	10:11am
BAR	Pass	10:11am
BT	Pass	10:11am

Blank Tests

Test	Status	Time
AIR	Pass	10:12am


Printer Tests

Test	Status	Time
PRNT	Pass	10:12am

CRC Tests

Test	Status	Time
COMP	Pass	10:12am
CAL	Pass	10:12am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Clay

Instrument Location Clay Co. Jail

Instrument Serial No. 008608

Hayesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of March, 20 19 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



David R. Cuth
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLAY COUNTY CLAY COUNTY JAIL 210

Serial Number: 008608
Test Date: 03/01/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: CUTLER, DANIEL R
Permit Number: 08457E
Effective:
09/01/2017-09/01/2019

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG716202
Exp Date: 06/11/2019

Test	g/210L	Time
DIAG	Pass	9:10am
AIR BLK	.00	9:11am
ACCY CHK	.07	9:12am
AIR BLK	.00	9:13am
SUB TEST	.00	9:13am
AIR BLK	.00	9:15am
SUB TEST	.00	9:16am
AIR BLK	.00	9:17am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

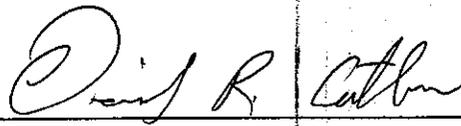

Analyst

Intox EC/IR-II: Preventive Maintenance

CLAY COUNTY CLAY COUNTY JAIL 210

Serial Number: 008608 Test Record Number: 1214
Test Date: 03/01/2019 Test Time: 9:18am EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:19am
FLO	Pass	9:19am
FC	Pass	9:19am

Temperature Tests

Test	Status	Time
FC1	Pass	9:19am
SRC	Pass	9:19am
DET	Pass	9:19am
BAR	Pass	9:19am
BT	Pass	9:19am

Blank Tests

Test	Status	Time
AIR	Pass	9:19am

Printer Tests

Test	Status	Time
PRNT	Pass	9:19am

CRC Tests

Test	Status	Time
COMP	Pass	9:20am
CAL	Pass	9:20am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II


County Cleveland Instrument Location Cleveland County SO - Arroy

Instrument Serial No. 008893 407 Mc Brayer St., Shelby

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLEVELAND COUNTY CLEVELAND SD-ANNEX
220

Serial Number: 008893
Test Date: 03/08/2019

Citation Number: M0000000-0

Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: HAYS, MARK D
Permit Number: 15924E
Effective:
01/01/2018-01/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG814902
Exp Date: 05/29/2020


Test	g/210L	Time
DIAG	Pass	9:49am
AIR BLK	.00	9:50am
ACCY CHK	.08	9:50am
AIR BLK	.00	9:51am
SUB TEST	.00	9:52am
AIR BLK	.00	9:53am
SUB TEST	.00	9:54am
AIR BLK	.00	9:55am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

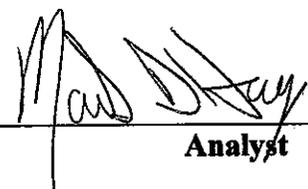

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CLEVELAND COUNTY CLEVELAND SD-ANNEX 220

Serial Number: 008893 Test Record Number: 1681
Test Date: 03/08/2019 Test Time: 9:56am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:56am
FLO	Pass	9:56am
FC	Pass	9:57am

Temperature Tests

Test	Status	Time
FC1	Pass	9:57am
SRC	Pass	9:57am
DET	Pass	9:57am
BAR	Pass	9:57am
BT	Pass	9:57am

Blank Tests

Test	Status	Time
AIR	Pass	9:57am


Printer Tests

Test	Status	Time
PRNT	Pass	9:57am

CRC Tests

Test	Status	Time
COMP	Pass	9:57am
CAL	Pass	9:57am

Preventive Maintenance
Status: Pass

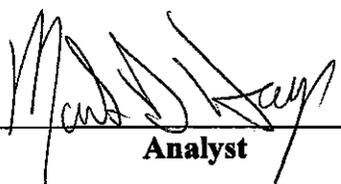

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II


County Columbus Instrument Location DAT mobile units

Instrument Serial No. 8616 Clarkston, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY BAT MOBILE UNIT 5 230

Serial Number: 008616 Test Record Number: 2455
Test Date: 03/16/2019 Test Time: 8:33pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:33pm
FLO	Pass	8:33pm
FC	Pass	8:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:33pm
SRC	Pass	8:33pm
DET	Pass	8:33pm
BAR	Pass	8:33pm
BT	Pass	8:33pm

Blank Tests

Test	Status	Time
AIR	Pass	8:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:34pm

CRC Tests

Test	Status	Time
COMP	Pass	8:34pm
CAL	Pass	8:34pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY BAT MOBILE UNIT 5 230

Serial Number: 008616
Test Date: 03/16/2019

Citation Number: M0000000-0
Subject's Name: NONE, NONE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: TODD, SHANE C
Permit Number: 11391E
Effective:
07/27/2018-07/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG807101
Exp Date: 03/12/2020

Test	g/210L	Time
DIAG	Pass	8:25pm
AIR BLK	.00	8:26pm
ACCY CHK	.07	8:27pm
AIR BLK	.00	8:28pm
SUB TEST	.00	8:28pm
AIR BLK	.00	8:29pm
SUB TEST	.00	8:31pm
AIR BLK	.00	8:32pm

Reported AC: .00 g/210L

Shane C Todd
Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Columbus Instrument Location BAT Mobile Unit #5

Instrument Serial No. 8707 Clarkton, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY BAT MOBILE UNIT 5 230

Serial Number: 008707 Test Record Number: 2570
Test Date: 03/16/2019 Test Time: 8:28pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:28pm
FLO	Pass	8:28pm
FC	Pass	8:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:29pm
SRC	Pass	8:29pm
DET	Pass	8:29pm
BAR	Pass	8:29pm
BT	Pass	8:29pm

Blank Tests

Test	Status	Time
AIR	Pass	8:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:29pm

CRC Tests

Test	Status	Time
COMP	Pass	8:30pm
CAL	Pass	8:30pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY BAT MOBILE UNIT 5 230

Serial Number: 008707
Test Date: 03/16/2019

Citation Number: M0000000-0
Subject's Name: NONE, NONE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: TODD, SHANE C
Permit Number: 11391E
Effective:
07/27/2018-07/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG807101
Exp Date: 03/12/2020

Test	g/210L	Time
DIAG	Pass	8:20pm
AIR BLK	.00	8:21pm
ACCY CHK	.08	8:22pm
AIR BLK	.00	8:23pm
SUB TEST	.00	8:24pm
AIR BLK	.00	8:24pm
SUB TEST	.00	8:26pm
AIR BLK	.00	8:27pm

Reported AC: .00 g/210L

Shane C. Todd
Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Duplin Instrument Location Wallace
Instrument Serial No. 008901 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



K.C. Rhodes
Signature of Certifying Official

601
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DUPLIN COUNTY WALLACE PD 300

Serial Number: 008901
Test Date: 03/06/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: RHODES, KENNETH C
Permit Number: 5329E
Effective:
05/01/2017-05/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG831801
Exp Date: 11/14/2020

Test	g/210L	Time
DIAG	Pass	11:21am
AIR BLK	.00	11:22am
ACCY CHK	.08	11:22am
AIR BLK	.00	11:23am
SUB TEST	.00	11:24am
AIR BLK	.00	11:25am
SUB TEST	.00	11:27am
AIR BLK	.00	11:28am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

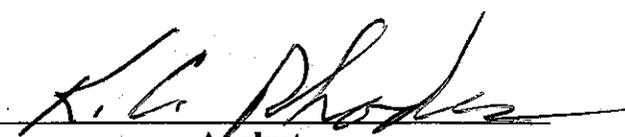
Analyst

Intox EC/IR-II: Preventive Maintenance

DUPLIN COUNTY WALLACE PD 300

Serial Number: 008901 Test Record Number: 1147
Test Date: 03/06/2019 Test Time: 11:30am EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:30am
FLO	Pass	11:30am
FC	Pass	11:30am

Temperature Tests

Test	Status	Time
FC1	Pass	11:31am
SRC	Pass	11:31am
DET	Pass	11:31am
BAR	Pass	11:31am
BT	Pass	11:31am

Blank Tests

Test	Status	Time
AIR	Pass	11:31am


Printer Tests

Test	Status	Time
PRNT	Pass	11:31am

CRC Tests

Test	Status	Time
COMP	Pass	11:31am
CAL	Pass	11:31am

Preventive Maintenance
Status: Pass

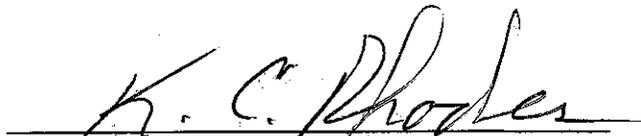

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Durham

Instrument Location Durham Co Jail


Instrument Serial No. 008859

219 S. Mangum ST Durham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of March, 20 19, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alex Barnes

Signature of Certifying Official

662

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008859
Test Date: 03/11/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, STOKES

Permit Number: 11434E

Effective:

05/01/2017-05/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG902106

Exp Date: 01/21/2021

Test	g/210L	Time
DIAG	Pass	9:57am
AIR BLK	.00	9:57am
ACCY CHK	.08	9:58am
AIR BLK	.00	9:59am
SUB TEST	.00	10:01am
AIR BLK	.00	10:02am
SUB TEST	.00	10:03am
AIR BLK	.00	10:04am

Reported AC: .00 g/210L

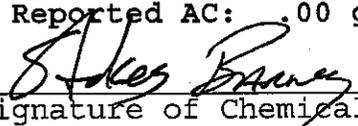

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008859 Test Record Number: 2257
Test Date: 03/11/2019 Test Time: 10:05am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:06am
FLO	Pass	10:06am
FC	Pass	10:06am

Temperature Tests

Test	Status	Time
FC1	Pass	10:06am
SRC	Pass	10:06am
DET	Pass	10:06am
BAR	Pass	10:06am
BT	Pass	10:06am

Blank Tests

Test	Status	Time
AIR	Pass	10:07am


Printer Tests

Test	Status	Time
PRNT	Pass	10:07am

CRC Tests

Test	Status	Time
COMP	Pass	10:07am
CAL	Pass	10:07am

Preventive Maintenance
Status: Pass

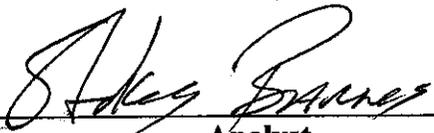

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Durham

Instrument Location Durham Co Jail


Instrument Serial No. 008891

219 S. Mangum St Durham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

662

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008891
Test Date: 03/11/2019

Citation Number: M0000000-0
Subject's Name:

~~PREVENTIVE, MAINTENANCE~~

Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, STOKES
Permit Number: 11434E
Effective:
05/01/2017-05/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG902106
Exp Date: 01/21/2021

Test	g/210L	Time
DIAG	Pass	9:56am
AIR BLK	.00	9:57am
ACCY CHK	.08	9:58am
AIR BLK	.00	9:59am
SUB TEST	.00	10:01am
AIR BLK	.00	10:02am
SUB TEST	.00	10:03am
AIR BLK	.00	10:04am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008891 Test Record Number: 4032
Test Date: 03/11/2019 Test Time: 10:05am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:06am
FLO	Pass	10:06am
FC	Pass	10:06am

Temperature Tests

Test	Status	Time
FC1	Pass	10:06am
SRC	Pass	10:06am
DET	Pass	10:06am
BAR	Pass	10:06am
BT	Pass	10:06am

Blank Tests

Test	Status	Time
AIR	Pass	10:07am

Printer Tests

Test	Status	Time
PRNT	Pass	10:07am

CRC Tests

Test	Status	Time
COMP	Pass	10:07am
CAL	Pass	10:07am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Durham

Instrument Location Durham Co JAIL

Instrument Serial No. 008878

219 S. Mangum St Durham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of March, 20 19, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

662

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008878
Test Date: 03/11/2019

Citation Number: M0000000-0
Subject's Name:

~~PREVENTIVE, MAINTENANCE~~

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, STOKES

Permit Number: 11434E

Effective:

05/01/2017-05/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG902106

Exp Date: 01/21/2021

Test	g/210L	Time
DIAG	Pass	9:55am
AIR BLK	.00	9:56am
ACCY CHK	.07	9:57am
AIR BLK	.00	9:58am
SUB TEST	.00	10:01am
AIR BLK	.00	10:01am
SUB TEST	.00	10:03am
AIR BLK	.00	10:04am

Reported AC: .00 g/210L

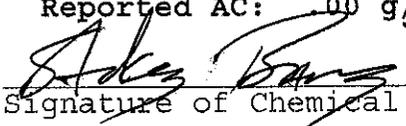
Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008878 Test Record Number: 4397
Test Date: 03/11/2019 Test Time: 10:05am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:05am
FLO	Pass	10:05am
FC	Pass	10:05am

Temperature Tests

Test	Status	Time
FC1	Pass	10:05am
SRC	Pass	10:05am
DET	Pass	10:05am
BAR	Pass	10:05am
BT	Pass	10:05am

Blank Tests

Test	Status	Time
AIR	Pass	10:06am


Printer Tests

Test	Status	Time
PRNT	Pass	10:06am

CRC Tests

Test	Status	Time
COMP	Pass	10:06am
CAL	Pass	10:06am

Preventive Maintenance
Status: Pass

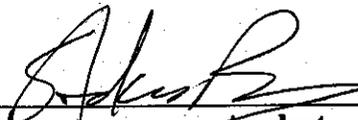

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County DURHAM

Instrument Location DURHAM CO. JAIL

Instrument Serial No. 008738

219 S. MANSON ST. DURHAM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of MARCH, 20 19 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bruce D. Smith
Signature of Certifying Official

637
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008738
Test Date: 03/28/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: SMITH, BRIAN D
Permit Number: 08937E
Effective:
08/01/2017-08/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG902106
Exp Date: 01/21/2021

Test	g/210L	Time
DIAG	Pass	3:45pm
AIR BLK	.00	3:45pm
ACCY CHK	.07	3:46pm
AIR BLK	.00	3:47pm
SUB TEST	.00	3:47pm
AIR BLK	.00	3:48pm
SUB TEST	.00	3:50pm
AIR BLK	.00	3:51pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008738 Test Record Number: 859

Test Date: 03/28/2019 Test Time: 3:52pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:52pm
FLO	Pass	3:52pm
FC	Pass	3:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:52pm
SRC	Pass	3:52pm
DET	Pass	3:52pm
BAR	Pass	3:52pm
BT	Pass	3:52pm

Blank Tests

Test	Status	Time
AIR	Pass	3:53pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:53pm

CRC Tests

Test	Status	Time
COMP	Pass	3:53pm
CAL	Pass	3:53pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Edgecombe Instrument Location Edgecombe Co. Magistrate's
Instrument Serial No. 008603 Office, 300 S. Anaconda Rd., Tarboro, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Key M. P.
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR
320

Serial Number: 008603
Test Date: 03/19/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GUARD, KELLY G

Permit Number: 12955E

Effective:

06/01/2017-06/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG821801


Exp Date: 08/06/2020

Test	g/210L	Time
DIAG	Pass	9:05am
AIR BLK	.00	9:06am
ACCY CHK	.08	9:07am
AIR BLK	.00	9:08am
SUB TEST	.00	9:09am
AIR BLK	.00	9:10am
SUB TEST	.00	9:11am
AIR BLK	.00	9:12am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR 320

Serial Number: 008603 Test Record Number: 1745
Test Date: 03/19/2019 Test Time: 9:13am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:14am
FLO	Pass	9:14am
FC	Pass	9:14am

Temperature Tests

Test	Status	Time
FC1	Pass	9:14am
SRC	Pass	9:14am
DET	Pass	9:14am
BAR	Pass	9:14am
BT	Pass	9:14am

Blank Tests

Test	Status	Time
AIR	Pass	9:14am


Printer Tests

Test	Status	Time
PRNT	Pass	9:14am

CRC Tests

Test	Status	Time
COMP	Pass	9:15am
CAL	Pass	9:15am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Edgecombe Instrument Location Edgecombe Co. Magistrate's

Instrument Serial No. 008663 Office, 3005. Anacanda Rd, Tarboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Kelly O

Signature of Certifying Official

643

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR
320

Serial Number: 008663
Test Date: 03/19/2019

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: GUARD, KELLY G
Permit Number: 12955E
Effective:
06/01/2017-06/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG721401
Exp Date: 08/02/2019


Test	g/210L	Time
DIAG	Pass	9:19am
AIR BLK	.00	9:20am
ACCY CHK	.08	9:20am
AIR BLK	.00	9:21am
SUB TEST	.00	9:22am
AIR BLK	.00	9:23am
SUB TEST	.00	9:25am
AIR BLK	.00	9:25am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR 320

Serial Number: 008663 Test Record Number: 3061
Test Date: 03/19/2019 Test Time: 9:28am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:28am
FLO	Pass	9:28am
FC	Pass	9:28am

Temperature Tests

Test	Status	Time
FC1	Pass	9:28am
SRC	Pass	9:28am
DET	Pass	9:28am
BAR	Pass	9:28am
BT	Pass	9:28am

Blank Tests

Test	Status	Time
AIR	Pass	9:29am

Printer Tests

Test	Status	Time
PRNT	Pass	9:29am

CRC Tests

Test	Status	Time
COMP	Pass	9:29am
CAL	Pass	9:29am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Gaston

Instrument Location Gaston County SO

Instrument Serial No. 008643

425 N. Marietta St., Gastonia

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

656

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: 008643

Test Date: 03/12/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HAYS, MARK D

Permit Number: 15924E

Effective:

01/01/2018-01/01/2020

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG807101

Exp Date: 03/12/2020


Test	g/210L	Time
DIAG	Pass	9:06am
AIR BLK	.00	9:07am
ACCY CHK	.07	9:07am
AIR BLK	.00	9:08am
SUB TEST	.00	9:09am
AIR BLK	.00	9:10am
SUB TEST	.00	9:11am
AIR BLK	.00	9:12am

Reported AC: 00 g/210L

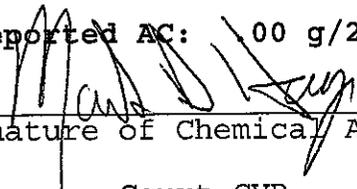

Signature of Chemical Analyst

Court CVR

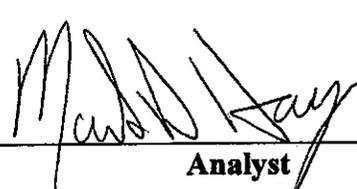

Analyst

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: 008643 Test Record Number: 3210
Test Date: 03/12/2019 Test Time: 9:14am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:14am
FLO	Pass	9:14am
FC	Pass	9:14am

Temperature Tests

Test	Status	Time
FC1	Pass	9:14am
SRC	Pass	9:14am
DET	Pass	9:14am
BAR	Pass	9:14am
BT	Pass	9:14am

Blank Tests

Test	Status	Time
AIR	Pass	9:15am


Printer Tests

Test	Status	Time
PRNT	Pass	9:15am

CRC Tests

Test	Status	Time
COMP	Pass	9:15am
CAL	Pass	9:15am

Preventive Maintenance
Status: Pass

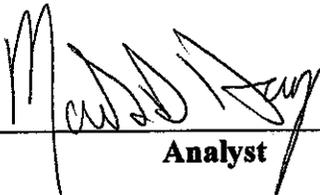

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II


County Gaston Instrument Location Bat Mobile Unit 1

Instrument Serial No. 008788

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Cheryl Joy
Signature of Certifying Official

658
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GASTON BAT MOBILE UNIT 1 350

Serial Number: 008788

Test Date: 03/16/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: TOWERY, CHAD V

Permit Number: 26632E

Effective:

06/01/2017-06/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG716201

Exp Date: 06/11/2019


Test	g/210L	Time
DIAG	Pass	5:17pm
AIR BLK	.00	5:18pm
ACCY CHK	.08	5:18pm
AIR BLK	.00	5:19pm
SUB TEST	.00	5:20pm
AIR BLK	.00	5:21pm
SUB TEST	.00	5:22pm
AIR BLK	.00	5:23pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GASTON BAT MOBILE UNIT 1 350

Serial Number: 008788 Test Record Number: 1382
Test Date: 03/16/2019 Test Time: 5:24pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:24pm
FLO	Pass	5:24pm
FC	Pass	5:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:24pm
SRC	Pass	5:24pm
DET	Pass	5:24pm
BAR	Pass	5:24pm
BT	Pass	5:24pm

Blank Tests

Test	Status	Time
AIR	Pass	5:25pm


Printer Tests

Test	Status	Time
PRNT	Pass	5:25pm

CRC Tests

Test	Status	Time
COMP	Pass	5:25pm
CAL	Pass	5:25pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County GATES Instrument Location GATES CO. S.D.

Instrument Serial No. 008884 202 COURT ST. GATESVILLE, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Linda A. Kess
Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GATES COUNTY GATES CO SO 360

Serial Number: 008884
Test Date: 03/20/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: KEESLER, LINDA
Permit Number: 11646E
Effective:
08/01/2017-08/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG814901
Exp Date: 05/29/2020


Test	g/210L	Time
DIAG	Pass	12:34pm
AIR BLK	.00	12:34pm
ACCY CHK	.08	12:35pm
AIR BLK	.00	12:36pm
SUB TEST	.00	12:37pm
AIR BLK	.00	12:38pm
SUB TEST	.00	12:39pm
AIR BLK	.00	12:40pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

GATES COUNTY GATES CO SO 360

Serial Number: 008884 Test Record Number: 893
Test Date: 03/20/2019 Test Time: 12:41pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:41pm
FLO	Pass	12:41pm
FC	Pass	12:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:41pm
SRC	Pass	12:41pm
DET	Pass	12:41pm
BAR	Pass	12:41pm
BT	Pass	12:41pm

Blank Tests

Test	Status	Time
AIR	Pass	12:42pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:42pm

CRC Tests

Test	Status	Time
COMP	Pass	12:42pm
CAL	Pass	12:42pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Granville Instrument Location Oxford PD

Instrument Serial No. 008924 204 E. McClanahan St. Oxford NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of MARCH, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

GRANVILLE COUNTY OXFORD PD 380

Serial Number: 008924 Test Record Number: 1426
Test Date: 03/18/2019 Test Time: 9:50am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:50am
FLO	Pass	9:50am
FC	Pass	9:50am

Temperature Tests

Test	Status	Time
FC1	Pass	9:50am
SRC	Pass	9:50am
DET	Pass	9:50am
BAR	Pass	9:50am
BT	Pass	9:50am

Blank Tests

Test	Status	Time
AIR	Pass	9:51am

Printer Tests

Test	Status	Time
PRNT	Pass	9:51am

CRC Tests

Test	Status	Time
COMP	Pass	9:51am
CAL	Pass	9:51am

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

GRANVILLE COUNTY OXFORD PD 380

Serial Number: 008924
Test Date: 03/18/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, STOKES
Permit Number: 11434E
Effective:
05/01/2017-05/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG821801
Exp Date: 08/06/2020


Test	g/210L	Time
DIAG	Pass	9:43am
AIR BLK	.00	9:44am
ACCY CHK	.08	9:44am
AIR BLK	.00	9:45am
SUB TEST	.00	9:46am
AIR BLK	.00	9:47am
SUB TEST	.00	9:48am
AIR BLK	.00	9:49am

Reported AC: 00 g/210L



Signature of Chemical Analyst

Court CVR

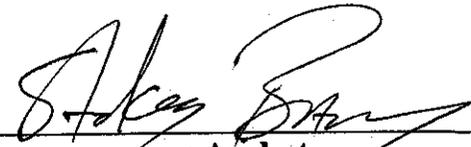

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Guilford Instrument Location Pat mobile Unit 4
Instrument Serial No. 008929 Guilford CO 50

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Janya B Skinner
Signature of Certifying Official

4211
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GREENSBORO BAT MOBILE UNIT 4 400

Serial Number: 008929
Test Date: 03/28/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Female
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: SKINNER, TONYA B
Permit Number: 13651E
Effective:
08/01/2017-08/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG814901
Exp Date: 05/29/2020

Test	g/210L	Time
DIAG	Pass	9:52pm
AIR BLK	.00	9:53pm
ACCY CHK	.08	9:54pm
AIR BLK	.00	9:55pm
SUB TEST	.00	9:56pm
AIR BLK	.00	9:57pm
SUB TEST	.00	9:59pm
AIR BLK	.00	10:00pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

GREENSBORO BAT MOBILE UNIT 4 400

Serial Number: 008929 Test Record Number: 1040
Test Date: 03/28/2019 Test Time: 10:01pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:02pm
FLO	Pass	10:02pm
FC	Pass	10:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:02pm
SRC	Pass	10:02pm
DET	Pass	10:02pm
BAR	Pass	10:02pm
BT	Pass	10:02pm

Blank Tests

Test	Status	Time
AIR	Pass	10:03pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:03pm

CRC Tests

Test	Status	Time
COMP	Pass	10:03pm
CAL	Pass	10:03pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Guilford

Instrument Location Bat Mobile Unit 4

Instrument Serial No. 008734

Guilford CO 50

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Donya B Skumin
Signature of Certifying Official

644
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GREENSBORO BAT MOBILE UNIT 4 400

Serial Number: 008736
Test Date: 03/28/2019

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Female

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: SKINNER, TONYA B

Permit Number: 13651E

Effective:

08/01/2017-08/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG716201


Exp Date: 06/11/2019

Test	g/210L	Time
DIAG	Pass	10:11pm
AIR BLK	.00	10:12pm
ACCY CHK	.07	10:12pm
AIR BLK	.00	10:13pm
SUB TEST	.00	10:14pm
AIR BLK	.00	10:15pm
SUB TEST	.00	10:18pm
AIR BLK	.00	10:19pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Subject Test

GREENSBORO BAT MOBILE UNIT 4 400

Serial Number: 008736

Test Date: 03/28/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Female

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: SKINNER, TONYA B

Permit Number: 13651E

Effective:

08/01/2017-08/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG716201

Exp Date: 06/11/2019

Test g/210L Time

DIAG Pass 9:45pm

AIR BLK .** 9:47pm

HIGH BLANK

Signature of Chemical Analyst

Court CVR

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Harrett Instrument Location BAT mobile Unit 1
Instrument Serial No. 008898 Leats PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of March, 20 19 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

660
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HARNETT COUNTY BAT MOBILE UNIT 1 420

Serial Number: 008898
Test Date: 03/22/2019

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: SMITH, JASON R

Permit Number: 19145E

Effective:

03/01/2018-03/01/2020

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG902201

Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	9:22pm
AIR BLK	.00	9:23pm
ACCY CHK	.08	9:24pm
AIR BLK	.00	9:25pm
SUB TEST	.00	9:25pm
AIR BLK	.00	9:26pm
SUB TEST	.00	9:28pm
AIR BLK	.00	9:29pm

Reported AC: .00 g/210L

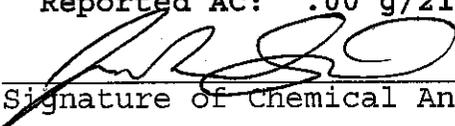

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HARNETT COUNTY BAT MOBILE UNIT 1 420

Serial Number: 008898 Test Record Number: 991
Test Date: 03/22/2019 Test Time: 9:39pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:39pm
FLO	Pass	9:39pm
FC	Pass	9:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:39pm
SRC	Pass	9:39pm
DET	Pass	9:39pm
BAR	Pass	9:39pm
BT	Pass	9:39pm

Blank Tests

Test	Status	Time
AIR	Pass	9:40pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:40pm

CRC Tests

Test	Status	Time
COMP	Pass	9:40pm
CAL	Pass	9:40pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County HERTFORD Instrument Location Murfreesboro P.D.

Instrument Serial No. DD8906 115 E. Broad St., Murfreesboro, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of MARCH, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Linda Kessel
Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HERTFORD COUNTY MURFREESBORO PD 450

Serial Number: 008906
Test Date: 03/20/2019

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, LINDA

Permit Number: 11646E

Effective:

08/01/2017-08/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG821401

Exp Date: 08/02/2020


Test	g/210L	Time
DIAG	Pass	11:32am
AIR BLK	.00	11:33am
ACCY CHK	.08	11:33am
AIR BLK	.00	11:35am
SUB TEST	.00	11:35am
AIR BLK	.00	11:36am
SUB TEST	.00	11:37am
AIR BLK	.00	11:38am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

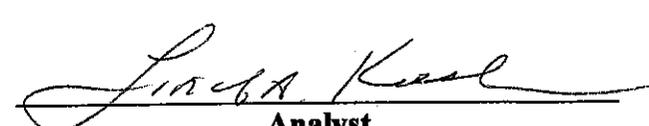

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HERTFORD COUNTY MURFREESBORO PD 450

Serial Number: 008906 Test Record Number: 704
Test Date: 03/20/2019 Test Time: 11:39am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:40am
FLO	Pass	11:40am
FC	Pass	11:40am

Temperature Tests

Test	Status	Time
FC1	Pass	11:40am
SRC	Pass	11:40am
DET	Pass	11:40am
BAR	Pass	11:40am
BT	Pass	11:40am

Blank Tests

Test	Status	Time
AIR	Pass	11:40am


Printer Tests

Test	Status	Time
PRNT	Pass	11:40am

CRC Tests

Test	Status	Time
COMP	Pass	11:41am
CAL	Pass	11:41am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County HEARTFORD Instrument Location Ahoskie P.D.
Instrument Serial No. 008848 705 W. Main St. Ahoskie, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of MARCH, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Linda Keel
Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HERTFORD COUNTY AHOSKIE PD 450

Serial Number: 008848
Test Date: 03/20/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, LINDA A

Permit Number: 11646E

Effective:

08/01/2017-08/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG821401

Exp Date: 08/02/2020


Test	g/210L	Time
DIAG	Pass	10:16am
AIR BLK	.00	10:17am
ACCY CHK	.07	10:18am
AIR BLK	.00	10:19am
SUB TEST	.00	10:20am
AIR BLK	.00	10:21am
SUB TEST	.00	10:22am
AIR BLK	.00	10:24am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HERTFORD COUNTY AHOSKIE PD 450

Serial Number: 008848 Test Record Number: 1394
Test Date: 03/20/2019 Test Time: 10:24am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:25am
FLO	Pass	10:25am
FC	Pass	10:25am

Temperature Tests

Test	Status	Time
FC1	Pass	10:25am
SRC	Pass	10:25am
DET	Pass	10:25am
BAR	Pass	10:25am
BT	Pass	10:25am

Blank Tests

Test	Status	Time
AIR	Pass	10:26am


Printer Tests

Test	Status	Time
PRNT	Pass	10:26am

CRC Tests

Test	Status	Time
COMP	Pass	10:26am
CAL	Pass	10:26am

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Iredell Instrument Location Mooreville PD
Instrument Serial No. 008685 950 W. Iredell Ave., Mooreville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



M. D. Hays
Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008685
Test Date: 03/19/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: HAYS, MARK D
Permit Number: 15924E
Effective:
01/01/2018-01/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG807102
Exp Date: 03/12/2020

Test	g/210L	Time
DIAG	Pass	8:44am
AIR BLK	.00	8:45am
ACCY CHK	.08	8:46am
AIR BLK	.00	8:47am
SUB TEST	.00	8:48am
AIR BLK	.00	8:48am
SUB TEST	.00	8:50am
AIR BLK	.00	8:51am

Reported AC: .00 g/210L

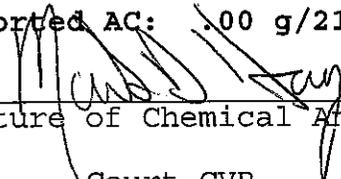

Signature of Chemical Analyst
Court CVR

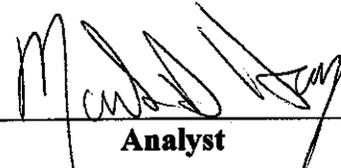

Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008685 Test Record Number: 3142
Test Date: 03/19/2019 Test Time: 8:54am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:55am
FLO	Pass	8:55am
FC	Pass	8:55am

Temperature Tests

Test	Status	Time
FC1	Pass	8:55am
SRC	Pass	8:55am
DET	Pass	8:55am
BAR	Pass	8:55am
BT	Pass	8:55am

Blank Tests

Test	Status	Time
AIR	Pass	8:55am


Printer Tests

Test	Status	Time
PRNT	Pass	8:55am

CRC Tests

Test	Status	Time
COMP	Pass	8:56am
CAL	Pass	8:56am

Preventive Maintenance
Status: Pass

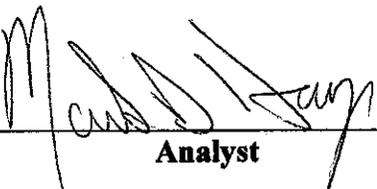

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Jackson Instrument Location Jackson Co. Jail

Instrument Serial No. 008722 Sylva, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



David R. Cuthbert
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JACKSON COUNTY JACKSON COUNTY JAIL 490

Serial Number: 008722
Test Date: 03/22/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: CUTLER, DANIEL R
Permit Number: 08457E
Effective:
09/01/2017-09/01/2019

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG734102
Exp Date: 12/07/2019

Test	g/210L	Time
DIAG	Pass	12:40pm
AIR BLK	.00	12:41pm
ACCY CHK	.07	12:42pm
AIR BLK	.00	12:43pm
SUB TEST	.00	12:44pm
AIR BLK	.00	12:45pm
SUB TEST	.00	12:46pm
AIR BLK	.00	12:47pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

JACKSON COUNTY JACKSON COUNTY JAIL 490

Serial Number: 008722 Test Record Number: 1091
Test Date: 03/22/2019 Test Time: 12:48pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:49pm
FLO	Pass	12:49pm
FC	Pass	12:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:49pm
SRC	Pass	12:49pm
DET	Pass	12:49pm
BAR	Pass	12:49pm
BT	Pass	12:49pm

Blank Tests

Test	Status	Time
AIR	Pass	12:49pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:50pm

CRC Tests

Test	Status	Time
COMP	Pass	12:50pm
CAL	Pass	12:50pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Jackson Instrument Location Jackson Co. Jail
Instrument Serial No. 008708 Sylva, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Chris R. Cuth
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JACKSON COUNTY JACKSON COUNTY JAIL 490

Serial Number: 008708
Test Date: 03/22/2019

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: CUTLER, DANIEL R

Permit Number: 08457E

Effective:

09/01/2017-09/01/2019

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG722408


Exp Date: 08/12/2019

Test	g/210L	Time
DIAG	Pass	12:39pm
AIR BLK	.00	12:40pm
ACCY CHK	.08	12:41pm
AIR BLK	.00	12:42pm
SUB TEST	.00	12:42pm
AIR BLK	.00	12:43pm
SUB TEST	.00	12:45pm
AIR BLK	.00	12:46pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

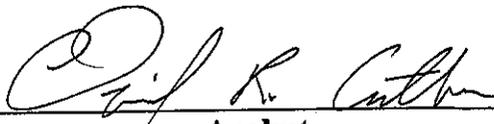

Analyst

Intox EC/IR-II: Preventive Maintenance

JACKSON COUNTY JACKSON COUNTY JAIL 490

Serial Number: 008708 Test Record Number: 1431
Test Date: 03/22/2019 Test Time: 12:47pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:47pm
FLO	Pass	12:47pm
FC	Pass	12:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:47pm
SRC	Pass	12:47pm
DET	Pass	12:47pm
BAR	Pass	12:47pm
BT	Pass	12:47pm

Blank Tests

Test	Status	Time
AIR	Pass	12:48pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:48pm

CRC Tests

Test	Status	Time
COMP	Pass	12:48pm
CAL	Pass	12:48pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Lee Co. Instrument Location Lee Co. Detention Center

Instrument Serial No. 002645 Say Road, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of MARCH, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LEE COUNTY DETENTION CENTER 520

Serial Number: 008645
Test Date: 03/04/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, GRAYHAM C

Permit Number: 07682E

Effective:

12/01/2017-12/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG716201


Exp Date: 06/11/2019

Test	g/210L	Time
DIAG	Pass	12:03pm
AIR BLK	.00	12:03pm
ACCY CHK	.07	12:04pm
AIR BLK	.00	12:05pm
SUB TEST	.00	12:05pm
AIR BLK	.00	12:06pm
SUB TEST	.00	12:08pm
AIR BLK	.00	12:08pm

Reported AC: .00 g/210L

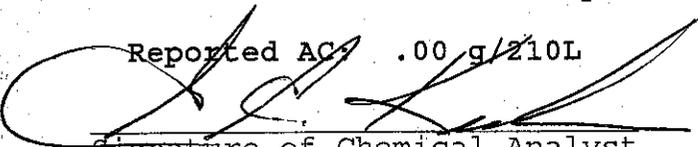
Signature of Chemical Analyst

Court CVR

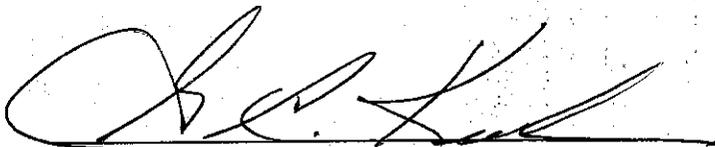
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

LEE COUNTY DETENTION CENTER 520

Serial Number: 008645 Test Record Number: 1925
Test Date: 03/04/2019 Test Time: 12:10pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:10pm
FLO	Pass	12:10pm
FC	Pass	12:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:10pm
SRC	Pass	12:10pm
DET	Pass	12:10pm
BAR	Pass	12:10pm
BT	Pass	12:10pm

Blank Tests

Test	Status	Time
AIR	Pass	12:11pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:11pm

CRC Tests

Test	Status	Time
COMP	Pass	12:11pm
CAL	Pass	12:11pm

Preventive Maintenance
Status: Pass

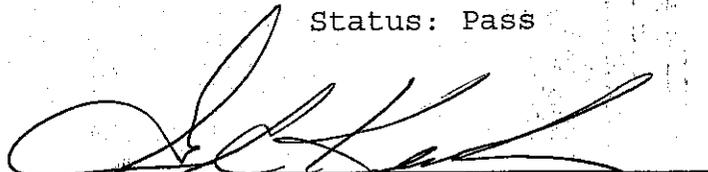

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Lee Co.

Instrument Location SANFORD Police Dept.

Instrument Serial No. 008867

SANFORD, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of MARCH, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LEE COUNTY SANFORD POLICE DEPT 520

Serial Number: 008867
Test Date: 03/04/2019

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: KEESLER, GRAYHAM C
Permit Number: 07682E
Effective:
12/01/2017-12/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG807102
Exp Date: 03/12/2020

Test	g/210L	Time
DIAG	Pass	11:11am
AIR BLK	.00	11:11am
ACCY CHK	.08	11:12am
AIR BLK	.00	11:13am
SUB TEST	.00	11:13am
AIR BLK	.00	11:14am
SUB TEST	.00	11:16am
AIR BLK	.00	11:17am

Reported AC: .00 g/210L

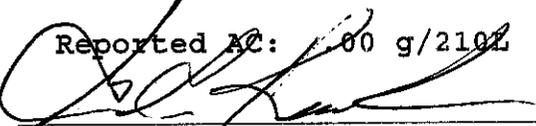
Signature of Chemical Analyst

Court CVR

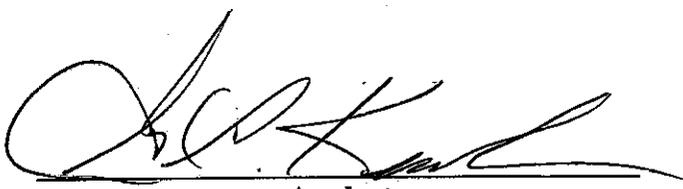
Analyst

Intox EC/IR-II: Preventive Maintenance

LEE COUNTY SANFORD POLICE DEPT 520

Serial Number: 008867 Test Record Number: 1096
Test Date: 03/04/2019 Test Time: 11:17am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:17am
FLO	Pass	11:17am
FC	Pass	11:18am

Temperature Tests

Test	Status	Time
FC1	Pass	11:18am
SRC	Pass	11:18am
DET	Pass	11:18am
BAR	Pass	11:18am
BT	Pass	11:18am

Blank Tests

Test	Status	Time
AIR	Pass	11:18am


Printer Tests

Test	Status	Time
PRNT	Pass	11:18am

CRC Tests

Test	Status	Time
COMP	Pass	11:18am
CAL	Pass	11:18am

Preventive Maintenance
Status: Pass

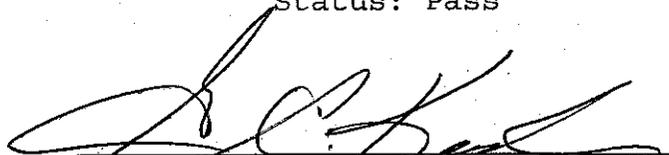

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Lenoir Instrument Location Lenoir Co. S.O.
Instrument Serial No. 008639 130 Queen St, Kinston, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LENOIR COUNTY LENOIR CO SO 530

Serial Number: 008639

Test Date: 03/12/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GUARD, KELLY G

Permit Number: 12955E

Effective:

06/01/2017-06/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG902201

Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	9:53am
AIR BLK	.00	9:54am
ACCY CHK	.07	9:55am
AIR BLK	.00	9:56am
SUB TEST	.00	9:56am
AIR BLK	.00	9:57am
SUB TEST	.00	9:59am
AIR BLK	.00	10:00am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY LENOIR CO SO 530

Serial Number: 008639 Test Record Number: 3268
Test Date: 03/12/2019 Test Time: 10:01am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:02am
FLO	Pass	10:02am
FC	Pass	10:02am

Temperature Tests

Test	Status	Time
FC1	Pass	10:02am
SRC	Pass	10:02am
DET	Pass	10:02am
BAR	Pass	10:02am
BT	Pass	10:02am

Blank Tests

Test	Status	Time
AIR	Pass	10:03am

Printer Tests

Test	Status	Time
PRNT	Pass	10:03am

CRC Tests

Test	Status	Time
COMP	Pass	10:03am
CAL	Pass	10:03am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Macon

Instrument Location Macon Co. Magistrate


Instrument Serial No. 008795

Highlands, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Daniel R. Calk

Signature of Certifying Official

635

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MACON COUNTY MACON CO MAGISTRATE 550

Serial Number: 008795

Test Date: 03/06/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: CUTLER, DANIEL R

Permit Number: 08457E

Effective:

09/01/2017-09/01/2019

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG716201

Exp Date: 06/11/2019


Test: g/210L Time

DIAG	Pass	1:42pm
AIR BLK	.00	1:43pm
ACCY CHK	.07	1:44pm
AIR BLK	.00	1:45pm
SUB TEST	.00	1:45pm
AIR BLK	.00	1:46pm
SUB TEST	.00	1:48pm
AIR BLK	.00	1:49pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR II: Preventive Maintenance

MACON COUNTY MACON CO MAGISTRATE 550

Serial Number: 008795 Test Record Number: 464
Test Date: 03/06/2019 Test Time: 1:50pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:50pm
FLO	Pass	1:50pm
FC	Pass	1:50pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:50pm
SRC	Pass	1:50pm
DET	Pass	1:50pm
BAR	Pass	1:50pm
BT	Pass	1:50pm

Blank Tests

Test	Status	Time
AIR	Pass	1:51pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:51pm

CRC Tests

Test	Status	Time
COMP	Pass	1:51pm
CAL	Pass	1:51pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Madison Instrument Location Maris Hill PD

Instrument Serial No. 008582 Maris Hill, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MADISON COUNTY MARS HILL PD 560

Serial Number: 008582

Test Date: 03/28/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J

Permit Number: 11304E

Effective:

05/01/2017-05/01/2019

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG721401

Exp Date: 08/02/2019

Test	g/210L	Time
DIAG	Pass	1:51pm
AIR BLK	.00	1:52pm
ACCY CHK	.08	1:53pm
AIR BLK	.00	1:54pm
SUB TEST	.00	1:54pm
AIR BLK	.00	1:55pm
SUB TEST	.00	1:57pm
AIR BLK	.00	1:58pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MADISON COUNTY MARS HILL PD 560

Serial Number: 008582 Test Record Number: 1141
Test Date: 03/28/2019 Test Time: 1:58pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	1:59pm
FLO	Pass	1:59pm
FC	Pass	1:59pm

Temperature Tests

Test	Status	Time
FCI	Pass	1:59pm
SRC	Pass	1:59pm
DET	Pass	1:59pm
BAR	Pass	1:59pm
BT	Pass	1:59pm

Blank Tests

Test	Status	Time
AIR	Pass	2:00pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:00pm

CRC Tests

Test	Status	Time
COMP	Pass	2:00pm
CAL	Pass	2:00pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County MARTIN Instrument Location MARTIN CO. S.O.

Instrument Serial No. 008912 305 E. MAIN ST., WILLIAMSTON, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of MARCH, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jacob A. Kessel
Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MARTIN COUNTY SHERIFF'S OFFICE 570

Serial Number: 008912
Test Date: 03/21/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: KEESLER, LINDA
Permit Number: 11646E
Effective:
08/01/2017-08/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG814901
Exp Date: 05/29/2020


Test	g/210L	Time
DIAG	Pass	1:18pm
AIR BLK	.00	1:19pm
ACCY CHK	.08	1:20pm
AIR BLK	.00	1:21pm
SUB TEST	.00	1:21pm
AIR BLK	.00	1:22pm
SUB TEST	.00	1:23pm
AIR BLK	.00	1:24pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MARTIN COUNTY SHERIFF'S OFFICE 570

Serial Number: 008912 Test Record Number: 1477
Test Date: 03/21/2019 Test Time: 1:25pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:25pm
FLO	Pass	1:25pm
FC	Pass	1:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:25pm
SRC	Pass	1:25pm
DET	Pass	1:25pm
BAR	Pass	1:25pm
BT	Pass	1:25pm

Blank Tests

Test	Status	Time
AIR	Pass	1:26pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:26pm

CRC Tests

Test	Status	Time
COMP	Pass	1:26pm
CAL	Pass	1:26pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County McDowell Instrument Location McDowell Co Jail

Instrument Serial No. 008892 Marion, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MCDOWELL COUNTY JAIL 580

Serial Number: 008892

Test Date: 03/05/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J

Permit Number: 11304E

Effective:

05/01/2017-05/01/2019

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG821401


Exp Date: 08/02/2020

Test	g/210L	Time
DIAG	Pass	2:29pm
AIR BLK	.00	2:30pm
ACCY CHK	.08	2:30pm
AIR BLK	.00	2:31pm
SUB TEST	.00	2:32pm
AIR BLK	.00	2:33pm
SUB TEST	.00	2:34pm
AIR BLK	.00	2:35pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MCDOWELL COUNTY JAIL 580

Serial Number: 008892 Test Record Number: 711
Test Date: 03/05/2019 Test Time: 2:36pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:37pm
FLO	Pass	2:37pm
FC	Pass	2:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:37pm
SRC	Pass	2:37pm
DET	Pass	2:37pm
BAR	Pass	2:37pm
BT	Pass	2:37pm

Blank Tests

Test	Status	Time
AIR	Pass	2:38pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:38pm

CRC Tests

Test	Status	Time
COMP	Pass	2:38pm
CAL	Pass	2:38pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County McDowell Instrument Location McDowell Co Jail
Instrument Serial No. 008898 Marion, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MCDOWELL COUNTY JAIL 580

Serial Number: 008888

Test Date: 03/05/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J

Permit Number: 11304E

Effective:

05/01/2017-05/01/2019

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG805801


Exp Date: 02/27/2020

Test	g/210L	Time
DIAG	Pass	2:29pm
AIR BLK	.00	2:30pm
ACCY CHK	.07	2:31pm
AIR BLK	.00	2:32pm
SUB TEST	.00	2:33pm
AIR BLK	.00	2:34pm
SUB TEST	.00	2:35pm
AIR BLK	.00	2:36pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MCDOWELL COUNTY JAIL 580

Serial Number: 008888 Test Record Number: 1515
Test Date: 03/05/2019 Test Time: 2:37pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:37pm
FLO	Pass	2:37pm
FC	Pass	2:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:38pm
SRC	Pass	2:38pm
DET	Pass	2:38pm
BAR	Pass	2:38pm
BT	Pass	2:38pm

Blank Tests

Test	Status	Time
AIR	Pass	2:38pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:38pm

CRC Tests

Test	Status	Time
COMP	Pass	2:38pm
CAL	Pass	2:38pm

Preventive Maintenance
Status: Pass

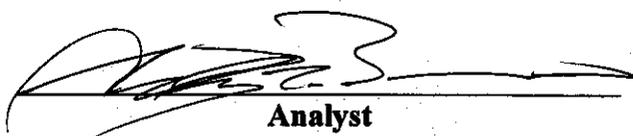

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Mecklenburg Instrument Location Huntersville PD
Instrument Serial No. 008747 9630 Julian Clark Ave. Huntersville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG HUNTERSVILLE PD 590

Serial Number: 008747
Test Date: 03/01/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HAYS, MARK D

Permit Number: 15924E

Effective:

01/01/2018-01/01/2020

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG722408

Exp Date: 08/12/2019


Test	g/210L	Time
DIAG	Pass	9:06am
AIR BLK	.00	9:07am
ACCY CHK	.08	9:07am
AIR BLK	.00	9:08am
SUB TEST	.00	9:09am
AIR BLK	.00	9:10am
SUB TEST	.00	9:12am
AIR BLK	.00	9:13am

Reported AC: .00 g/210L

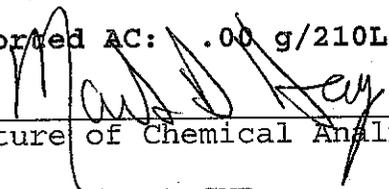

Signature of Chemical Analyst

Court CVR

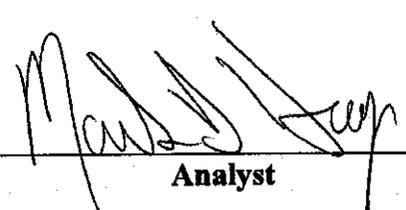

Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG HUNTERSVILLE PD 590

Serial Number: 008747 Test Record Number: 2706
Test Date: 03/01/2019 Test Time: 9:14am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:14am
FLO	Pass	9:14am
FC	Pass	9:14am

Temperature Tests

Test	Status	Time
FC1	Pass	9:14am
SRC	Pass	9:14am
DET	Pass	9:14am
BAR	Pass	9:14am
BT	Pass	9:14am

Blank Tests

Test	Status	Time
AIR	Pass	9:15am

Printer Tests

Test	Status	Time
PRNT	Pass	9:15am

CRC Tests

Test	Status	Time
COMP	Pass	9:15am
CAL	Pass	9:15am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Mecklenburg Instrument Location Matthews PD
Instrument Serial No. 008699 1201 Crews Rd, Matthews

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14th day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hill
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY MATTHEWS PD 590

Serial Number: 008699
Test Date: 03/14/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HUTCHINSON, JOSEPH E

Permit Number: 19951E

Effective:

08/01/2017-08/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG710701


Exp Date: 04/17/2019

Test	g/210L	Time
DIAG	Pass	4:02pm
AIR BLK	.00	4:03pm
ACCY CHK	.07	4:03pm
AIR BLK	.00	4:04pm
SUB TEST	.00	4:05pm
AIR BLK	.00	4:06pm
SUB TEST	.00	4:07pm
AIR BLK	.00	4:09pm

Reported AC: .00 g/210L

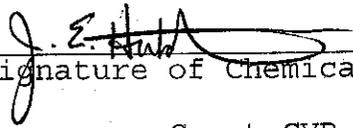
Signature of Chemical Analyst

Court CVR

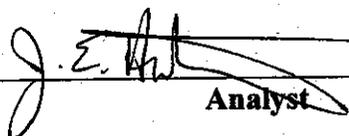
Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY MATTHEWS PD 590

Serial Number: 008699 Test Record Number: 2744
Test Date: 03/14/2019 Test Time: 4:10pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	4:10pm
FLO	Pass	4:10pm
FC	Pass	4:10pm

Temperature Tests

Test	Status	Time
FCI	Pass	4:10pm
SRC	Pass	4:10pm
DET	Pass	4:10pm
BAR	Pass	4:10pm
BT	Pass	4:10pm

Blank Tests

Test	Status	Time
AIR	Pass	4:11pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:11pm

CRC Tests

Test	Status	Time
COMP	Pass	4:11pm
CAL	Pass	4:11pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Moore Co. Instrument Location Southern Pines P.D.

Instrument Serial No. 008120 Southern Pines, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MOORE COUNTY SOUTHERN PINES PD 620

Serial Number: 008720
Test Date: 03/19/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, GRAYHAM C

Permit Number: 07682E

Effective:

12/01/2017-12/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG805802


Exp Date: 02/27/2020

Test	g/210L	Time
DIAG	Pass	1:32pm
AIR BLK	.00	1:33pm
ACCY CHK	.07	1:34pm
AIR BLK	.00	1:34pm
SUB TEST	.00	1:35pm
AIR BLK	.00	1:36pm
SUB TEST	.00	1:37pm
AIR BLK	.00	1:38pm

Reported AG: .00 g/210L

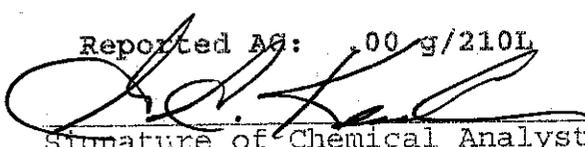
Signature of Chemical Analyst

Court CVR

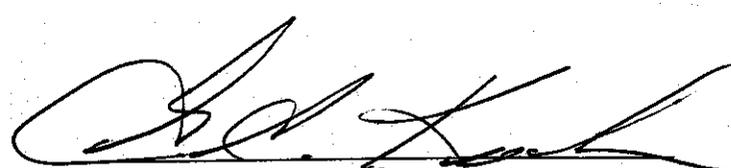
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MOORE COUNTY SOUTHERN PINES PD 620

Serial Number: 008720 Test Record Number: 1102
Test Date: 03/19/2019 Test Time: 1:39pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	1:39pm
FLO	Pass	1:39pm
FC	Pass	1:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:39pm
SRC	Pass	1:39pm
DET	Pass	1:39pm
BAR	Pass	1:39pm
BT	Pass	1:39pm

Blank Tests

Test	Status	Time
AIR	Pass	1:40pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:40pm

CRC Tests

Test	Status	Time
COMP	Pass	1:40pm
CAL	Pass	1:40pm

Preventive Maintenance
Status: Pass

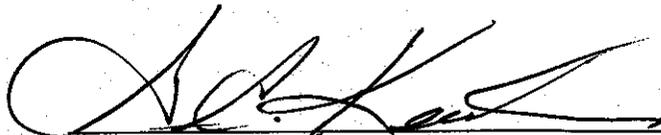

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Moore Co. Instrument Location Pinehurst Police Dept.

Instrument Serial No. 008110 Pinehurst, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MOORE COUNTY PINEHURST PD 620

Serial Number: 008710
Test Date: 03/19/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, GRAYHAM C

Permit Number: 07682E

Effective:

12/01/2017-12/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG821401

Exp Date: 08/02/2020

Test	g/210L	Time
DIAG	Pass	12:37pm
AIR BLK	.00	12:37pm
ACCY CHK	.07	12:38pm
AIR BLK	.00	12:39pm
SUB TEST	.00	12:39pm
AIR BLK	.00	12:40pm
SUB TEST	.00	12:42pm
AIR BLK	.00	12:43pm

Reported AC: .00 g/210L

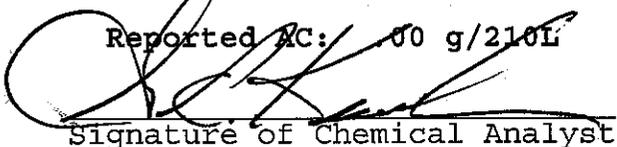
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MOORE COUNTY PINEHURST PD 620

Serial Number: 008710 Test Record Number: 1586
Test Date: 03/19/2019 Test Time: 12:43pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:43pm
FLO	Pass	12:43pm
FC	Pass	12:44pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:44pm
SRC	Pass	12:44pm
DET	Pass	12:44pm
BAR	Pass	12:44pm
BT	Pass	12:44pm

Blank Tests

Test	Status	Time
AIR	Pass	12:44pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:44pm

CRC Tests

Test	Status	Time
COMP	Pass	12:45pm
CAL	Pass	12:45pm

Preventive Maintenance
Status: Pass

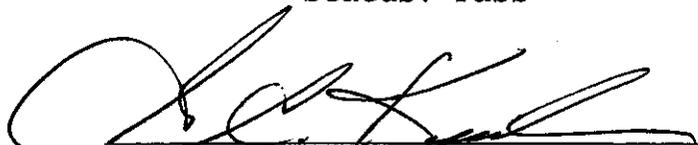

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Moore Co. Instrument Location Moore Co. Detention Center

Instrument Serial No. 008735 CARThage, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MOORE COUNTY DETENTION CENTER 620

Serial Number: 008735
Test Date: 03/19/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: KEESLER, GRAYHAM C.
Permit Number: 07682E
Effective:
12/01/2017-12/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG805802
Exp Date: 02/27/2020

Test	g/210L	Time
DIAG	Pass	11:45am
AIR BLK	.00	11:45am
ACCY CHK	.08	11:46am
AIR BLK	.00	11:47am
SUB TEST	.00	11:48am
AIR BLK	.00	11:49am
SUB TEST	.00	11:50am
AIR BLK	.00	11:51am

Reported AC: .00 g/210L

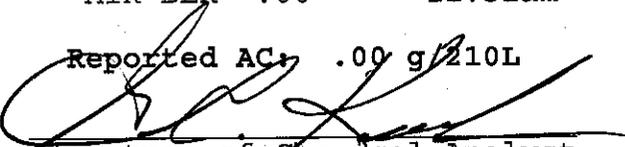
Signature of Chemical Analyst

Court CVR

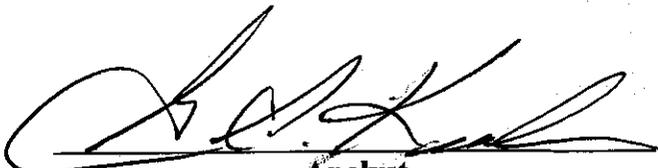
Analyst

Intox EC/IR-II: Preventive Maintenance

MOORE COUNTY DETENTION CENTER 620

Serial Number: 008735 Test Record Number: 2233
Test Date: 03/19/2019 Test Time: 11:52am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:52am
FLO	Pass	11:52am
FC	Pass	11:52am

Temperature Tests

Test	Status	Time
FC1	Pass	11:52am
SRC	Pass	11:52am
DET	Pass	11:52am
BAR	Pass	11:52am
BT	Pass	11:52am

Blank Tests

Test	Status	Time
AIR	Pass	11:53am


Printer Tests

Test	Status	Time
PRNT	Pass	11:53am

CRC Tests

Test	Status	Time
COMP	Pass	11:53am
CAL	Pass	11:53am

Preventive Maintenance
Status: Pass

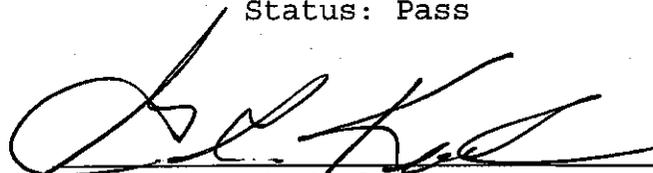

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County New Hanover Instrument Location BAT Mobile unit #5
Instrument Serial No. 8704 William Law, Inc.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEWHANOVER COUNTY BAT MOBILE UNIT 5
640

Serial Number: 008704
Test Date: 03/15/2019

Citation Number: M0000000-0
Subject's Name: NONE, NONE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: TODD, SHANE C
Permit Number: 11391E
Effective:
07/27/2018-07/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG807101
Exp Date: 03/12/2020

Test	g/210L	Time
DIAG	Pass	10:56pm
AIR BLK	.00	10:57pm
ACCY CHK	.08	10:58pm
AIR BLK	.00	10:59pm
SUB TEST	.00	10:59pm
AIR BLK	.00	11:00pm
SUB TEST	.00	11:02pm
AIR BLK	.00	11:03pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

NEWHANOVER COUNTY BAT MOBILE UNIT 5 640

Serial Number: 008704 Test Record Number: 539
Test Date: 03/15/2019 Test Time: 11:20pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:20pm
FLO	Pass	11:20pm
FC	Pass	11:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:21pm
SRC	Pass	11:21pm
DET	Pass	11:21pm
BAR	Pass	11:21pm
BT	Pass	11:21pm

Blank Tests

Test	Status	Time
AIR	Pass	11:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:21pm

CRC Tests

Test	Status	Time
COMP	Pass	11:21pm
CAL	Pass	11:21pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County New Hanover Instrument Location BAT Mobile unit #5
Instrument Serial No. 8707 Wilmington, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of March, 20 19, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

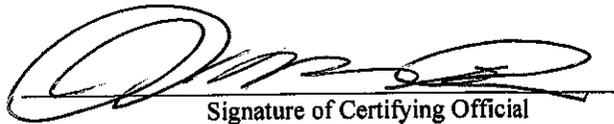


Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

NEWHANOVER COUNTY BAT MOBILE UNIT 5 640

Serial Number: 008707 Test Record Number: 2568
Test Date: 03/15/2019 Test Time: 11:02pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:02pm
FLO	Pass	11:02pm
FC	Pass	11:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:02pm
SRC	Pass	11:02pm
DET	Pass	11:02pm
BAR	Pass	11:02pm
BT	Pass	11:02pm

Blank Tests

Test	Status	Time
AIR	Pass	11:03pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:03pm

CRC Tests

Test	Status	Time
COMP	Pass	11:03pm
CAL	Pass	11:03pm

Preventive Maintenance
Status: Pass

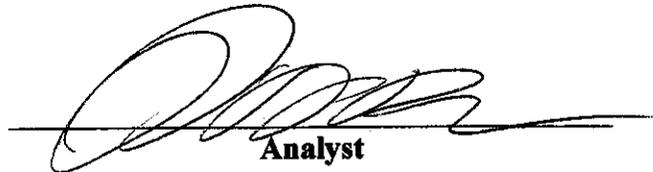
Analyst

Intox EC/IR-II: Subject Test

NEWHANOVER COUNTY BAT MOBILE UNIT 5
640

Serial Number: 008707
Test Date: 03/15/2019

Citation Number: M0000000-0
Subject's Name: NONE, NONE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: TODD, SHANE C
Permit Number: 11391E
Effective:
07/27/2018-07/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG807101
Exp Date: 03/12/2020

Test	g/210L	Time
DIAG	Pass	10:53pm
AIR BLK	.00	10:54pm
ACCY CHK	.08	10:55pm
AIR BLK	.00	10:56pm
SUB TEST	.00	10:57pm
AIR BLK	.00	10:57pm
SUB TEST	.00	10:59pm
AIR BLK	.00	11:00pm

Reported AC: .00 g/210L

Shane C. Todd
Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II


County New Hanover Instrument Location BAT Mobile unit #5


Instrument Serial No. 8575 Wilmington

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of March, 20 19, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



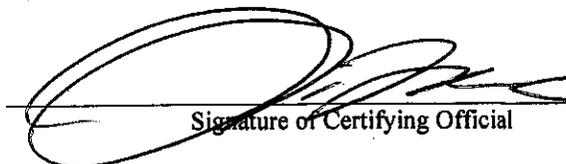
Signature of Certifying Official 664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

NEWHANOVER COUNTY BAT MOBILE UNIT 5 640

Serial Number: 008575 Test Record Number: 1137
Test Date: 03/15/2019 Test Time: 11:01pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:01pm
FLO	Pass	11:01pm
FC	Pass	11:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:01pm
SRC	Pass	11:01pm
DET	Pass	11:01pm
BAR	Pass	11:01pm
BT	Pass	11:01pm

Blank Tests

Test	Status	Time
AIR	Pass	11:02pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:02pm

CRC Tests

Test	Status	Time
COMP	Pass	11:02pm
CAL	Pass	11:02pm

Preventive Maintenance
Status: Pass

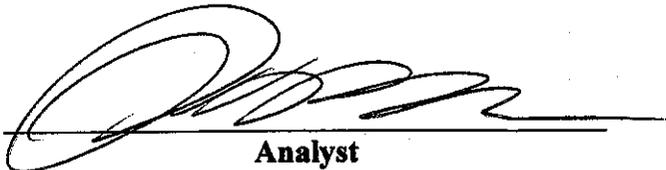

Analyst

Intox EC/IR-II: Subject Test

NEWHANOVER COUNTY BAT MOBILE UNIT 5
640

Serial Number: 008575
Test Date: 03/15/2019

Citation Number: M0000000-0
Subject's Name: NONE, NONE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: TODD, SHANE C
Permit Number: 11391E
Effective:
07/27/2018-07/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG807101
Exp Date: 03/12/2020

Test	g/210L	Time
DIAG	Pass	10:48pm
AIR BLK	.00	10:49pm
ACCY CHK	.08	10:50pm
AIR BLK	.00	10:51pm
SUB TEST	.00	10:52pm
AIR BLK	.00	10:53pm
SUB TEST	.00	10:54pm
AIR BLK	.00	10:55pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County PERSON Instrument Location PERSON CO. LEC

Instrument Serial No. 008890 120 COURT ST. ROCKFORD, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of MARCH, 20 19 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bruce D. Smith
Signature of Certifying Official

637
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PERSON COUNTY PERSON CO. LEC 720

Serial Number: 008880

Test Date: 03/11/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: SMITH, BRIAN D

Permit Number: 08937E

Effective:

08/01/2017-08/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG821801

Exp Date: 08/06/2020


Test	g/210L	Time
DIAG	Pass	12:29pm
AIR BLK	.00	12:30pm
ACCY CHK	.08	12:31pm
AIR BLK	.00	12:32pm
SUB TEST	.00	12:32pm
AIR BLK	.00	12:33pm
SUB TEST	.00	12:35pm
AIR BLK	.00	12:36pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

PERSON COUNTY PERSON CO. LEC 720

Serial Number: 008880 Test Record Number: 1436
Test Date: 03/11/2019 Test Time: 12:36pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:37pm
FLO	Pass	12:37pm
FC	Pass	12:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:37pm
SRC	Pass	12:37pm
DET	Pass	12:37pm
BAR	Pass	12:37pm
BT	Pass	12:37pm

Blank Tests

Test	Status	Time
AIR	Pass	12:38pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:38pm

CRC Tests

Test	Status	Time
COMP	Pass	12:38pm
CAL	Pass	12:38pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County PERSON Instrument Location PERSON CD. LFC

Instrument Serial No. 008693 120 COURT ST. ROXBORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of MARCH, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



B. J. Smith
Signature of Certifying Official

637
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PERSON COUNTY PERSON CO. LEC 720

Serial Number: 008693
Test Date: 03/11/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: SMITH, BRIAN D
Permit Number: 08937E
Effective:
08/01/2017-08/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG821801
Exp Date: 08/06/2020


Test	g/210L	Time
DIAG	Pass	12:27pm
AIR BLK	.00	12:28pm
ACCY CHK	.07	12:29pm
AIR BLK	.00	12:30pm
SUB TEST	.00	12:30pm
AIR BLK	.00	12:31pm
SUB TEST	.00	12:33pm
AIR BLK	.00	12:33pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

PERSON COUNTY PERSON CO. LEC 720

Serial Number: 008693 Test Record Number: 1567
Test Date: 03/11/2019 Test Time: 12:34pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:34pm
FLO	Pass	12:34pm
FC	Pass	12:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:35pm
SRC	Pass	12:35pm
DET	Pass	12:35pm
BAR	Pass	12:35pm
BT	Pass	12:35pm

Blank Tests

Test	Status	Time
AIR	Pass	12:35pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:35pm

CRC Tests

Test	Status	Time
COMP	Pass	12:36pm
CAL	Pass	12:36pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Pitt Instrument Location Pitt Co Detention Center
Instrument Serial No. 0086608 124 Detention Dr., Greenville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008668
Test Date: 03/21/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: GUARD, KELLY G
Permit Number: 12955E
Effective:
06/01/2017-06/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG722408
Exp Date: 08/12/2019

Test	g/210L	Time
DIAG	Pass	9:13am
AIR BLK	.00	9:13am
ACCY CHK	.07	9:14am
AIR BLK	.00	9:15am
SUB TEST	.00	9:16am
AIR BLK	.00	9:16am
SUB TEST	.00	9:18am
AIR BLK	.00	9:19am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008668 Test Record Number: 3183
Test Date: 03/21/2019 Test Time: 9:20am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:20am
FLO	Pass	9:20am
FC	Pass	9:20am

Temperature Tests

Test	Status	Time
FC1	Pass	9:21am
SRC	Pass	9:21am
DET	Pass	9:21am
BAR	Pass	9:21am
BT	Pass	9:21am

Blank Tests

Test	Status	Time
AIR	Pass	9:21am

Printer Tests

Test	Status	Time
PRNT	Pass	9:21am

CRC Tests

Test	Status	Time
COMP	Pass	9:21am
CAL	Pass	9:21am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Pitt Instrument Location Pitt Co. Detention Center

Instrument Serial No. 00 8646 124 Detention Dr., Greenville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008646
Test Date: 03/21/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: GUARD, KELLY G
Permit Number: 12955E
Effective:
06/01/2017-06/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG902201
Exp Date: 01/22/2021


Test	g/210L	Time
DIAG	Pass	9:44am
AIR BLK	.00	9:45am
ACCY CHK	.08	9:45am
AIR BLK	.00	9:46am
SUB TEST	.00	9:47am
AIR BLK	.00	9:48am
SUB TEST	.00	9:49am
AIR BLK	.00	9:50am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008646 Test Record Number: 3831
Test Date: 03/21/2019 Test Time: 9:51am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:52am
FLO	Pass	9:52am
FC	Pass	9:52am

Temperature Tests

Test	Status	Time
FC1	Pass	9:52am
SRC	Pass	9:52am
DET	Pass	9:52am
BAR	Pass	9:52am
BT	Pass	9:52am

Blank Tests

Test	Status	Time
AIR	Pass	9:53am


Printer Tests

Test	Status	Time
PRNT	Pass	9:53am

CRC Tests

Test	Status	Time
COMP	Pass	9:53am
CAL	Pass	9:53am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County P. H. Instrument Location Pitt Co. Detention Center
Instrument Serial No. 008662 124 Detention Dr., Greenville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008662
Test Date: 03/21/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GUARD, KELLY G

Permit Number: 12955E

Effective:

06/01/2017-06/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG902201

Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	10:11am
AIR BLK	.00	10:12am
ACCY CHK	.08	10:12am
AIR BLK	.00	10:14am
SUB TEST	.00	10:14am
AIR BLK	.00	10:15am
SUB TEST	.00	10:17am
AIR BLK	.00	10:17am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008662 Test Record Number: 1105
Test Date: 03/21/2019 Test Time: 10:18am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:19am
FLO	Pass	10:19am
FC	Pass	10:19am

Temperature Tests

Test	Status	Time
FC1	Pass	10:19am
SRC	Pass	10:19am
DET	Pass	10:19am
BAR	Pass	10:19am
BT	Pass	10:19am

Blank Tests

Test	Status	Time
AIR	Pass	10:20am

Printer Tests

Test	Status	Time
PRNT	Pass	10:20am

CRC Tests

Test	Status	Time
COMP	Pass	10:20am
CAL	Pass	10:20am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Randolph Co. Instrument Location Liberty Police Dept.

Instrument Serial No. 008830 Liberty, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY LIBERTY PD 750

Serial Number: 008830
Test Date: 03/28/2019

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, GRAYHAM C

Permit Number: 07682E

Effective:

12/01/2017-12/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG902201


Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	1:07pm
AIR BLK	.00	1:08pm
ACCY CHK	.08	1:09pm
AIR BLK	.00	1:10pm
SUB TEST	.00	1:10pm
AIR BLK	.00	1:11pm
SUB TEST	.00	1:13pm
AIR BLK	.00	1:14pm

Reported AC: .00 g/210L

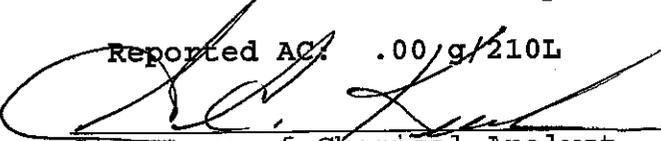
Signature of Chemical Analyst

Court CVR

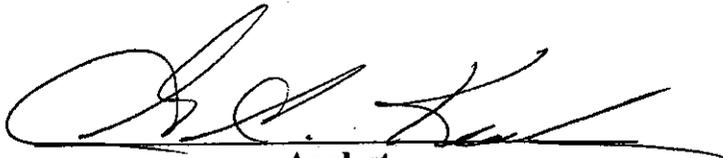
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY LIBERTY PD 750

Serial Number: 008830 Test Record Number: 623
Test Date: 03/28/2019 Test Time: 1:14pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:14pm
FLO	Pass	1:14pm
FC	Pass	1:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:15pm
SRC	Pass	1:15pm
DET	Pass	1:15pm
BAR	Pass	1:15pm
BT	Pass	1:15pm

Blank Tests

Test	Status	Time
AIR	Pass	1:15pm

Printer Tests


Test	Status	Time
PRNT	Pass	1:15pm

CRC Tests

Test	Status	Time
COMP	Pass	1:15pm
CAL	Pass	1:15pm

Preventive Maintenance

Status: Pass

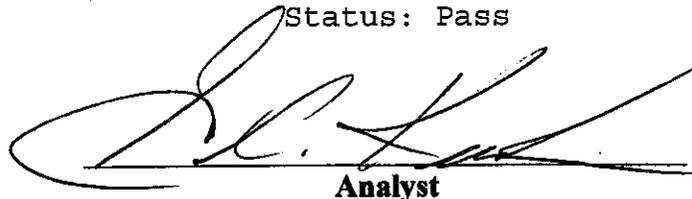

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Randolph Co. Instrument Location Randleman Police Dept.
Instrument Serial No. 008737 Randleman, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of MARCH, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY RANDLEMAN PD 750

Serial Number: 008737
Test Date: 03/28/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: KEESLER, GRAYHAM C
Permit Number: 07682E
Effective:
12/01/2017-12/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG902201
Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	12:01pm
AIR BLK	.00	12:02pm
ACCY CHK	.08	12:03pm
AIR BLK	.00	12:04pm
SUB TEST	.00	12:04pm
AIR BLK	.00	12:05pm
SUB TEST	.00	12:07pm
AIR BLK	.00	12:08pm

Reported AC: .00 g/210L

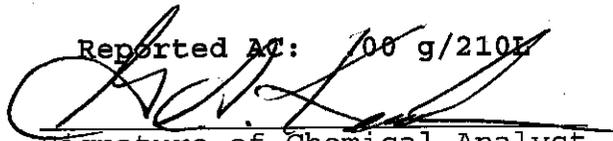
Signature of Chemical Analyst

Court CVR

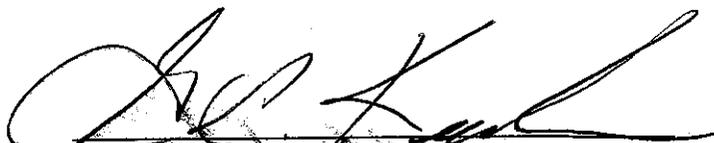
Analyst

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY RANDLEMAN PD 750

Serial Number: 008737 Test Record Number: 1086
Test Date: 03/28/2019 Test Time: 12:08pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:08pm
FLO	Pass	12:08pm
FC	Pass	12:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:08pm
SRC	Pass	12:08pm
DET	Pass	12:08pm
BAR	Pass	12:08pm
BT	Pass	12:08pm

Blank Tests

Test	Status	Time
AIR	Pass	12:09pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:09pm

CRC Tests

Test	Status	Time
COMP	Pass	12:09pm
CAL	Pass	12:09pm

Preventive Maintenance
Status: Pass

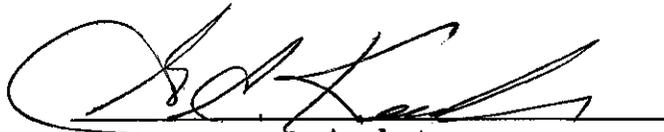

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County RICHMOND Instrument Location RICHMOND COUNTY

Instrument Serial No. 008701 MAGISTRATE'S OFFICE
ROCKINGHAM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of MARCH, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Barnes
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RICHMOND COUNTY MAGISTRATE'S OFFICE
760

Serial Number: 008701
Test Date: 03/20/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 15671E
Effective:
07/01/2017-07/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG902202
Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	10:52am
AIR BLK	.00	10:53am
ACCY CHK	.08	10:53am
AIR BLK	.00	10:54am
SUB TEST	.00	10:55am
AIR BLK	.00	10:56am
SUB TEST	.00	10:57am
AIR BLK	.00	10:58am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

RICHMOND COUNTY MAGISTRATE'S OFFICE 760

Serial Number: 008701 Test Record Number: 1182
Test Date: 03/20/2019 Test Time: 10:59am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:00am
FLO	Pass	11:00am
FC	Pass	11:00am

Temperature Tests

Test	Status	Time
FC1	Pass	11:00am
SRC	Pass	11:00am
DET	Pass	11:00am
BAR	Pass	11:00am
BT	Pass	11:00am

Blank Tests

Test	Status	Time
AIR	Pass	11:01am

Printer Tests

Test	Status	Time
PRNT	Pass	11:01am

CRC Tests

Test	Status	Time
COMP	Pass	11:01am
CAL	Pass	11:01am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County RICHMOND Instrument Location RICHMOND COUNTY

Instrument Serial No. 008840 MAGISTRATE'S OFFICE
ROCKINGHAM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of MARCH, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Barnes
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RICHMOND COUNTY MAGISTRATE'S OFFICE
760

Serial Number: 008840
Test Date: 03/20/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 15671E
Effective:
07/01/2017-07/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG902202
Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	10:51am
AIR BLK	.00	10:52am
ACCY CHK	.08	10:52am
AIR BLK	.00	10:54am
SUB TEST	.00	10:54am
AIR BLK	.00	10:55am
SUB TEST	.00	10:57am
AIR BLK	.00	10:58am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

RICHMOND COUNTY MAGISTRATE'S OFFICE 760

Serial Number: 008840 Test Record Number: 2257
Test Date: 03/20/2019 Test Time: 10:58am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:59am
FLO	Pass	10:59am
FC	Pass	10:59am

Temperature Tests

Test	Status	Time
FC1	Pass	10:59am
SRC	Pass	10:59am
DET	Pass	10:59am
BAR	Pass	10:59am
BT	Pass	10:59am

Blank Tests

Test	Status	Time
AIR	Pass	11:00am

Printer Tests

Test	Status	Time
PRNT	Pass	11:00am

CRC Tests

Test	Status	Time
COMP	Pass	11:00am
CAL	Pass	11:00am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Richmond Instrument Location BAT mobile unit #5
Instrument Serial No. 8616 Hawlet, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of March, 20 19, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

RICHMOND COUNTY BAT MOBILE UNIT 5 760

Serial Number: 008616 Test Record Number: 2458
Test Date: 03/22/2019 Test Time: 10:34pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:35pm
FLO	Pass	10:35pm
FC	Pass	10:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:35pm
SRC	Pass	10:35pm
DET	Pass	10:35pm
BAR	Pass	10:35pm
BT	Pass	10:35pm

Blank Tests

Test	Status	Time
AIR	Pass	10:36pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:36pm

CRC Tests

Test	Status	Time
COMP	Pass	10:36pm
CAL	Pass	10:36pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

RICHMOND COUNTY BAT MOBILE UNIT 5 760

Serial Number: 008616
Test Date: 03/22/2019

Citation Number: M0000000-0
Subject's Name: NONE, NONE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: TODD, SHANE C
Permit Number: 11391E
Effective:
07/27/2018-07/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG807101
Exp Date: 03/12/2020


Test	g/210L	Time
DIAG	Pass	10:19pm
AIR BLK	.00	10:20pm
ACCY CHK	.07	10:20pm
AIR BLK	.00	10:21pm
SUB TEST	.00	10:22pm
AIR BLK	.00	10:23pm
SUB TEST	.00	10:24pm
AIR BLK	.00	10:25pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

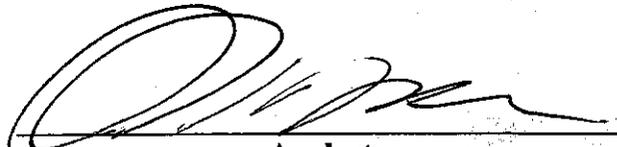

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Richmond Instrument Location BAT Mobile Unit #5
Instrument Serial No. 8570 Hunter, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

RICHMOND COUNTY BAT MOBILE UNIT 5 760

Serial Number: 008575 Test Record Number: 1140

Test Date: 03/22/2019 Test Time: 10:25pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:26pm
FLO	Pass	10:26pm
FC	Pass	10:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:26pm
SRC	Pass	10:26pm
DET	Pass	10:26pm
BAR	Pass	10:26pm
BT	Pass	10:26pm

Blank Tests

Test	Status	Time
AIR	Pass	10:27pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:27pm

CRC Tests

Test	Status	Time
COMP	Pass	10:27pm
CAL	Pass	10:27pm

Preventive Maintenance
Status: Pass


Analyst

Intox EC/IR-II: Subject Test

RICHMOND COUNTY BAT MOBILE UNIT 5 760

Serial Number: 008575
Test Date: 03/22/2019

Citation Number: M0000000-0
Subject's Name: NONE, NONE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: TODD, SHANE C
Permit Number: 11391E
Effective:
07/27/2018-07/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG807101
Exp Date: 03/12/2020

Test	g/210L	Time
DIAG	Pass	10:17pm
AIR BLK	.00	10:18pm
ACCY CHK	.08	10:18pm
AIR BLK	.00	10:19pm
SUB TEST	.00	10:20pm
AIR BLK	.00	10:21pm
SUB TEST	.00	10:22pm
AIR BLK	.00	10:23pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Richmond Instrument Location BAT mobile unit #5
Instrument Serial No. 008820 Hewlett, Inc.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of March, 20 19, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

RICHMOND COUNTY BAT MOBILE UNIT 5 760

Serial Number: 008826 Test Record Number: 8093
Test Date: 03/22/2019 Test Time: 10:34pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:34pm
FLO	Pass	10:34pm
FC	Pass	10:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:34pm
SRC	Pass	10:34pm
DET	Pass	10:34pm
BAR	Pass	10:34pm
BT	Pass	10:34pm

Blank Tests

Test	Status	Time
AIR	Pass	10:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:35pm

CRC Tests

Test	Status	Time
COMP	Pass	10:35pm
CAL	Pass	10:35pm

Preventive Maintenance
Status: Pass


Analyst

Intox EC/IR-II: Subject Test

RICHMOND COUNTY BAT MOBILE UNIT 5 760

Serial Number: 008826

Test Date: 03/22/2019

Citation Number: M0000000-0

Subject's Name: NONE, NONE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: TODD, SHANE C

Permit Number: 11391E

Effective:

07/27/2018-07/01/2020

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG807101

Exp Date: 03/12/2020

Test	g/210L	Time
DIAG	Pass	10:13pm
AIR BLK	.00	10:15pm
ACCY CHK	.08	10:15pm
AIR BLK	.00	10:16pm
SUB TEST	.00	10:17pm
AIR BLK	.00	10:18pm
SUB TEST	.00	10:19pm
AIR BLK	.00	10:20pm

Reported AC: .00 g/210L

Shane C. Todd

Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Richmond Instrument Location BAT Mobile Unit #5
Instrument Serial No. 8826 Rockingham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of March, 20 19, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

RICHMOND COUNTY BAT MOBILE UNIT 5 760

Serial Number: 008826 Test Record Number: 8095
Test Date: 03/23/2019 Test Time: 10:32pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:33pm
FLO	Pass	10:33pm
FC	Pass	10:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:33pm
SRC	Pass	10:33pm
DET	Pass	10:33pm
BAR	Pass	10:33pm
BT	Pass	10:33pm

Blank Tests

Test	Status	Time
AIR	Pass	10:34pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:34pm

CRC Tests

Test	Status	Time
COMP	Pass	10:34pm
CAL	Pass	10:34pm

Preventive Maintenance
Status: Pass

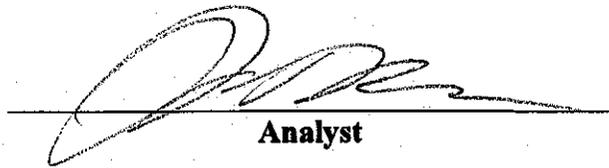

Analyst

Intox EC/IR-II: Subject Test

RICHMOND COUNTY BAT MOBILE UNIT 5 760

Serial Number: 008826
Test Date: 03/23/2019

Citation Number: M0000000-0
Subject's Name: NONE, NONE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: TODD, SHANE C
Permit Number: 11391E
Effective:
07/27/2018-07/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG807101
Exp Date: 03/12/2020

Test	g/210L	Time
DIAG	Pass	10:14pm
AIR BLK	.00	10:15pm
ACCY CHK	.08	10:16pm
AIR BLK	.00	10:17pm
SUB TEST	.00	10:17pm
AIR BLK	.00	10:18pm
SUB TEST	.00	10:20pm
AIR BLK	.00	10:21pm

Reported AC: .00 g/210L

Shane C. Todd
Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Richmond Instrument Location BAT mobile unit #5

Instrument Serial No. 8575 Rockingham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RICHMOND COUNTY BAT MOBILE UNIT 5 760

Serial Number: 008575
Test Date: 03/23/2019

Citation Number: M0000000-0
Subject's Name: NONE, NONE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: TODD, SHANE C
Permit Number: 11391E
Effective:
07/27/2018-07/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG807101
Exp Date: 03/12/2020

Test	g/210L	Time
DIAG	Pass	10:13pm
AIR BLK	.00	10:14pm
ACCY CHK	.08	10:15pm
AIR BLK	.00	10:16pm
SUB TEST	.00	10:16pm
AIR BLK	.00	10:17pm
SUB TEST	.00	10:19pm
AIR BLK	.00	10:20pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

RICHMOND COUNTY BAT MOBILE UNIT 5 760

Serial Number: 008575 Test Record Number: 1144
Test Date: 03/23/2019 Test Time: 10:33pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:33pm
FLO	Pass	10:33pm
FC	Pass	10:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:34pm
SRC	Pass	10:34pm
DET	Pass	10:34pm
BAR	Pass	10:34pm
BT	Pass	10:34pm

Blank Tests

Test	Status	Time
AIR	Pass	10:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:34pm

CRC Tests

Test	Status	Time
COMP	Pass	10:34pm
CAL	Pass	10:34pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Richmond Instrument Location BAT mobile unit #5
Instrument Serial No. 8616 Rockingham, Inc.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

RICHMOND COUNTY BAT MOBILE UNIT 5 760

Serial Number: 008616 Test Record Number: 2461
Test Date: 03/23/2019 Test Time: 10:27pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:28pm
FLO	Pass	10:28pm
FC	Pass	10:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:28pm
SRC	Pass	10:28pm
DET	Pass	10:28pm
BAR	Pass	10:28pm
BT	Pass	10:28pm

Blank Tests

Test	Status	Time
AIR	Pass	10:28pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:28pm

CRC Tests

Test	Status	Time
COMP	Pass	10:29pm
CAL	Pass	10:29pm

Preventive Maintenance
Status: Pass


Analyst

Intox EC/IR-II: Subject Test

RICHMOND COUNTY BAT MOBILE UNIT 5 760

Serial Number: 008616
Test Date: 03/23/2019

Citation Number: M0000000-0
Subject's Name: NONE, NONE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: TODD, SHANE C
Permit Number: 11391E
Effective:
07/27/2018-07/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG807101
Exp Date: 03/12/2020

Test	g/210L	Time
DIAG	Pass	10:15pm
AIR BLK	.00	10:16pm
ACCY CHK	.07	10:17pm
AIR BLK	.00	10:17pm
SUB TEST	.00	10:18pm
AIR BLK	.00	10:19pm
SUB TEST	.00	10:21pm
AIR BLK	.00	10:22pm

Reported AC: .00 g/210L

Shane C. Todd
Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Robeson Instrument Location BAT Mobile unit #5
Instrument Serial No. 8707 NC. Hwy 211 & Chicka Lumberton

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of March, 20 19 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008707

Test Date: 03/02/2019

Citation Number: M0000000-0

Subject's Name: NONE, NONE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: TODD, SHANE C

Permit Number: 11391E

Effective:

07/27/2018-07/01/2020

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG807101

Exp Date: 03/12/2020

Test	g/210L	Time
DIAG	Pass	7:09pm
AIR BLK	.00	7:10pm
ACCY CHK	.08	7:11pm
AIR BLK	.00	7:12pm
SUB TEST	.00	7:12pm
AIR BLK	.00	7:13pm
SUB TEST	.00	7:15pm
AIR BLK	.00	7:16pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008707 Test Record Number: 2563
Test Date: 03/02/2019 Test Time: 7:17pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:17pm
FLO	Pass	7:17pm
FC	Pass	7:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:17pm
SRC	Pass	7:17pm
DET	Pass	7:17pm
BAR	Pass	7:17pm
BT	Pass	7:17pm

Blank Tests

Test	Status	Time
AIR	Pass	7:18pm


Printer Tests

Test	Status	Time
PRNT	Pass	7:18pm

CRC Tests

Test	Status	Time
COMP	Pass	7:18pm
CAL	Pass	7:18pm

Preventive Maintenance
Status: Pass

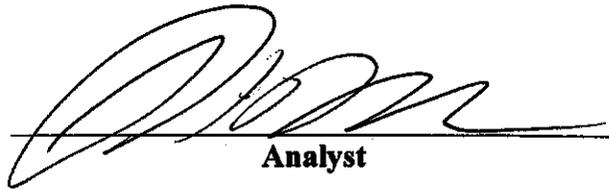

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Robeson Instrument Location BAT Mobile Unit #5

Instrument Serial No. 008616 NC 211 & Choke Rd. Lumberton

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of March, 20 19, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008616
Test Date: 03/02/2019

Citation Number: M0000000-0
Subject's Name: NONE, NONE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: TODD, SHANE C
Permit Number: 11391E
Effective:
07/27/2018-07/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG807101
Exp Date: 03/12/2020

Test	g/210L	Time
DIAG	Pass	7:48pm
AIR BLK	.00	7:49pm
ACCY CHK	.07	7:50pm
AIR BLK	.00	7:51pm
SUB TEST	.00	7:51pm
AIR BLK	.00	7:52pm
SUB TEST	.00	7:54pm
AIR BLK	.00	7:55pm

Reported AC: .00 g/210L

Shane C. Todd
Signature of Chemical Analyst

Court CVR

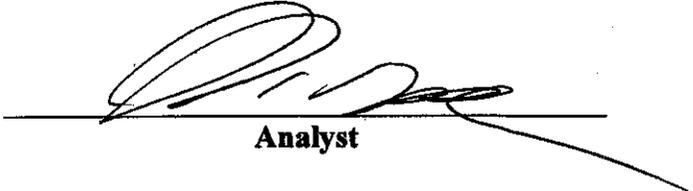
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008616 Test Record Number: 2452
Test Date: 03/02/2019 Test Time: 7:57pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:58pm
FLO	Pass	7:58pm
FC	Pass	7:58pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:58pm
SRC	Pass	7:58pm
DET	Pass	7:58pm
BAR	Pass	7:58pm
BT	Pass	7:58pm

Blank Tests

Test	Status	Time
AIR	Pass	7:59pm


Printer Tests

Test	Status	Time
PRNT	Pass	7:59pm

CRC Tests

Test	Status	Time
COMP	Pass	7:59pm
CAL	Pass	7:59pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Robeson Instrument Location BAT Mobile Unit #5
Instrument Serial No. 008826 N.C. 211 & Chicken Rd. Lumberton

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of March, 20 19, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008826 Test Record Number: 8091
Test Date: 03/02/2019 Test Time: 7:26pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:27pm
FLO	Pass	7:27pm
FC	Pass	7:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:27pm
SRC	Pass	7:27pm
DET	Pass	7:27pm
BAR	Pass	7:27pm
BT	Pass	7:27pm

Blank Tests

Test	Status	Time
AIR	Pass	7:28pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:28pm

CRC Tests

Test	Status	Time
COMP	Pass	7:28pm
CAL	Pass	7:28pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008826
Test Date: 03/02/2019

Citation Number: M0000000-0
Subject's Name: NONE, NONE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: TODD, SHANE C
Permit Number: 11391E
Effective:
07/27/2018-07/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG807101
Exp Date: 03/12/2020

Test	g/210L	Time
DIAG	Pass	7:14pm
AIR BLK	.00	7:15pm
ACCY CHK	.08	7:15pm
AIR BLK	.00	7:16pm
SUB TEST	.00	7:17pm
AIR BLK	.00	7:18pm
SUB TEST	.00	7:19pm
AIR BLK	.00	7:20pm

Reported AC: .00 g/210L

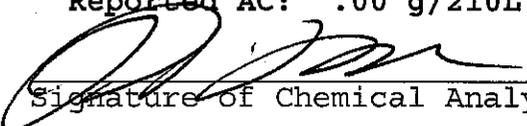
Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Rowan

Instrument Location China Grove

Instrument Serial No. 008862

Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Dale Farley
Signature of Certifying Official

655
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY CHINA GROVE PD 790

Serial Number: 008862
Test Date: 03/15/2019

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Female

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: FARLEY, CYNTHIA D

Permit Number: 24123E

Effective:

11/01/2018-11/01/2020

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG821401


Exp Date: 08/02/2020

Test	g/210L	Time
DIAG	Pass	1:34pm
AIR BLK	.00	1:34pm
ACCY CHK	.07	1:35pm
AIR BLK	.00	1:36pm
SUB TEST	.00	1:36pm
AIR BLK	.00	1:37pm
SUB TEST	.00	1:39pm
AIR BLK	.00	1:40pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

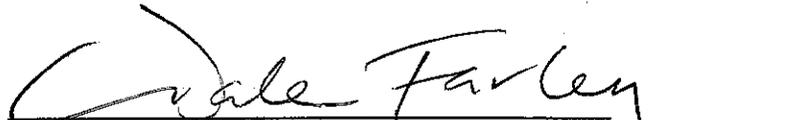
Analyst

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY CHINA GROVE PD 790

Serial Number: 008862 Test Record Number: 844
Test Date: 03/15/2019 Test Time: 1:41pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:41pm
FLO	Pass	1:41pm
FC	Pass	1:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:41pm
SRC	Pass	1:41pm
DET	Pass	1:41pm
BAR	Pass	1:41pm
BT	Pass	1:41pm

Blank Tests

Test	Status	Time
AIR	Pass	1:42pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:42pm

CRC Tests

Test	Status	Time
COMP	Pass	1:42pm
CAL	Pass	1:42pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Rutherford Instrument Location Forest City PD
Instrument Serial No. 0088889 187 S Church St., Forest City

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RUTHERFORD COUNTY FOREST CITY PD 800

Serial Number: 008889

Test Date: 03/08/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HAYS, MARK D

Permit Number: 15924E

Effective:

01/01/2018-01/01/2020

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG814902


Exp Date: 05/29/2020

Test	g/210L	Time
DIAG	Pass	10:43am
AIR BLK	.00	10:44am
ACCY CHK	.07	10:45am
AIR BLK	.00	10:46am
SUB TEST	.00	10:47am
AIR BLK	.00	10:48am
SUB TEST	.00	10:49am
AIR BLK	.00	10:50am

Reported AC: .00 g/210L

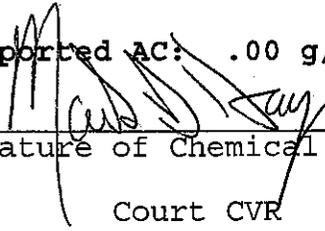

Signature of Chemical Analyst
Court CVR

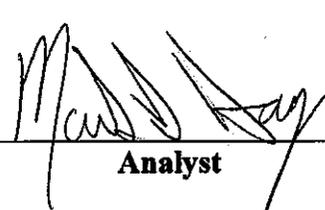

Analyst

Intox EC/IR-II: Preventive Maintenance

RUTHERFORD COUNTY FOREST CITY PD 800

Serial Number: 008889 Test Record Number: 832
Test Date: 03/08/2019 Test Time: 10:51am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:52am
FLO	Pass	10:52am
FC	Pass	10:52am

Temperature Tests

Test	Status	Time
FC1	Pass	10:52am
SRC	Pass	10:52am
DET	Pass	10:52am
BAR	Pass	10:52am
BT	Pass	10:52am

Blank Tests

Test	Status	Time
AIR	Pass	10:52am


Printer Tests

Test	Status	Time
PRNT	Pass	10:52am

CRC Tests

Test	Status	Time
COMP	Pass	10:53am
CAL	Pass	10:53am

Preventive Maintenance
Status: *Pass*

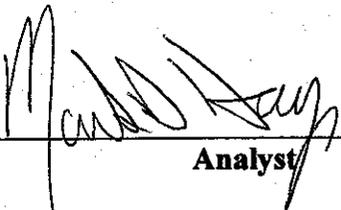

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Stokes Instrument Location King Police Department
Instrument Serial No. 008610

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

655
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STOKES COUNTY KING P D 840

Serial Number: 008610
Test Date: 03/21/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Female

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: FARLEY, CYNTHIA D

Permit Number: 24123E

Effective:

11/01/2018-11/01/2020

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG821401


Exp Date: 08/02/2020

Test	g/210L	Time
DIAG	Pass	12:44pm
AIR BLK	.00	12:45pm
ACCY CHK	.07	12:45pm
AIR BLK	.00	12:46pm
SUB TEST	.00	12:48pm
AIR BLK	.00	12:49pm
SUB TEST	.00	12:51pm
AIR BLK	.00	12:51pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

STOKES COUNTY KING P D 840

Serial Number: 008610 Test Record Number: 2026
Test Date: 03/21/2019 Test Time: 12:53pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:53pm
FLO	Pass	12:53pm
FC	Pass	12:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:53pm
SRC	Pass	12:53pm
DET	Pass	12:53pm
BAR	Pass	12:53pm
BT	Pass	12:53pm

Blank Tests

Test	Status	Time
AIR	Pass	12:54pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:54pm

CRC Tests

Test	Status	Time
COMP	Pass	12:54pm
CAL	Pass	12:54pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Surry Instrument Location Surry County Jail
Instrument Serial No. 008934 Dobson, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Dale Farley
Signature of Certifying Official

655
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SURRY COUNTY SURRY CO JAIL 850

Serial Number: 008934
Test Date: 03/20/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: *Female*
Driver's License State: *XX*
Driver's License Number: *NONE*


Analyst's Name: *FARLEY, CYNTHIA D*
Permit Number: *24123E*
Effective:
11/01/2018-11/01/2020

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG821401
Exp Date: 08/02/2020.



Test	g/210L	Time
DIAG	Pass	1:12pm
AIR BLK	.00	1:12pm
ACCY CHK	.07	1:13pm
AIR BLK	.00	1:14pm
SUB TEST	.00	1:15pm
AIR BLK	.00	1:16pm
SUB TEST	.00	1:18pm
AIR BLK	.00	1:19pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

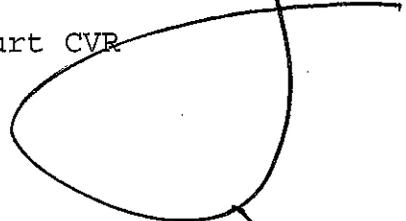Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY SURRY CO JAIL 850

Serial Number: 008934 Test Record Number: 2003
Test Date: 03/20/2019 Test Time: 1:20pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:20pm
FLO	Pass	1:20pm
FC	Pass	1:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:20pm
SRC	Pass	1:20pm
DET	Pass	1:20pm
BAR	Pass	1:20pm
BT	Pass	1:20pm

Blank Tests

Test	Status	Time
AIR	Pass	1:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:21pm

CRC Tests

Test	Status	Time
COMP	Pass	1:21pm
CAL	Pass	1:21pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Surry Instrument Location Mount Airy
Instrument Serial No. 008943 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



C. Dale Farley
Signature of Certifying Official

655
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SURRY COUNTY MOUNT AIRY PD 850

Serial Number: 008943
Test Date: 03/20/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENACE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Female
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: FARLEY, CYNTHIA D
Permit Number: 24123E
Effective:
11/01/2018-11/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG821401
Exp Date: 08/02/2020


Test	g/210L	Time
DIAG	Pass	2:42pm
AIR BLK	.00	2:42pm
ACCY CHK	.08	2:43pm
AIR BLK	.00	2:44pm
SUB TEST	.00	2:45pm
AIR BLK	.00	2:45pm
SUB TEST	.00	2:47pm
AIR BLK	.00	2:48pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

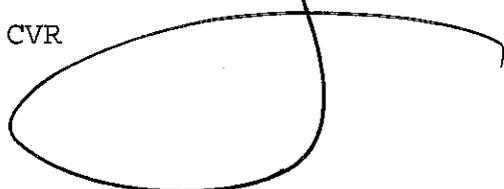



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY MOUNT AIRY PD 850

Serial Number: 008943 Test Record Number: 2091
Test Date: 03/20/2019 Test Time: 2:49pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:49pm
FLO	Pass	2:49pm
FC	Pass	2:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:49pm
SRC	Pass	2:49pm
DET	Pass	2:49pm
BAR	Pass	2:49pm
BT	Pass	2:49pm

Blank Tests

Test	Status	Time
AIR	Pass	2:50pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:50pm

CRC Tests

Test	Status	Time
COMP	Pass	2:50pm
CAL	Pass	2:50pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Surry Instrument Location Pilot Mountain
Instrument Serial No. 008938 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

655
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SURRY COUNTY PILOT MOUNTAIN PD 850

Serial Number: 008938

Test Date: 03/21/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Female

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: FARLEY, CYNTHIA D

Permit Number: 24123E

Effective:

11/01/2018-11/01/2020

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG734101

Exp Date: 12/07/2019

Test	g/210L	Time
DIAG	Pass	11:03am
AIR BLK	.00	11:03am
ACCY CHK	.07	11:04am
AIR BLK	.00	11:05am
SUB TEST	.00	11:07am
AIR BLK	.00	11:08am
SUB TEST	.00	11:10am
AIR BLK	.00	11:10am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY PILOT MOUNTAIN PD 850
Serial Number: 008938 Test Record Number: 632
Test Date: 03/21/2019 Test Time: 11:12am EDT
System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:12am
FLO	Pass	11:12am
FC	Pass	11:12am

Temperature Tests

Test	Status	Time
FC1	Pass	11:13am
SRC	Pass	11:13am
DET	Pass	11:13am
BAR	Pass	11:13am
BT	Pass	11:13am

Blank Tests

Test	Status	Time
AIR	Pass	11:13am

Printer Tests

Test	Status	Time
PRNT	Pass	11:13am

CRC Tests

Test	Status	Time
COMP	Pass	11:13am
CAL	Pass	11:13am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Transylvania Instrument Location Transylvania Co. Jail
Instrument Serial No. 008609 Brevard, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul R. Cuthbert
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

TRANSYLVANIA COUNTY TRANSYLVANIA CO
JAIL 870

Serial Number: 008609
Test Date: 03/20/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: CUTLER, DANIEL R
Permit Number: 08457E
Effective:
09/01/2017-09/01/2019

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG734102
Exp Date: 12/07/2019

Test	g/210L	Time
DIAG	Pass	1:57pm
AIR BLK	.00	1:58pm
ACCY CHK	.07	1:58pm
AIR BLK	.00	1:59pm
SUB TEST	.00	2:00pm
AIR BLK	.00	2:00pm
SUB TEST	.00	2:02pm
AIR BLK	.00	2:03pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

TRANSYLVANIA COUNTY TRANSYLVANIA CO JAIL 870

Serial Number: 008609 Test Record Number: 811
Test Date: 03/20/2019 Test Time: 2:03pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:04pm
FLO	Pass	2:04pm
FC	Pass	2:04pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:04pm
SRC	Pass	2:04pm
DET	Pass	2:04pm
BAR	Pass	2:04pm
BT	Pass	2:04pm

Blank Tests

Test	Status	Time
AIR	Pass	2:05pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:05pm

CRC Tests

Test	Status	Time
COMP	Pass	2:05pm
CAL	Pass	2:05pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Transylvania Instrument Location Transylvania Co. Jail
Instrument Serial No. 008820 Brevard, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul R. Cutler
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

TRANSYLVANIA COUNTY TRANSYLVANIA CO
JAIL 870

Serial Number: 008820
Test Date: 03/20/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: CUTLER, DANIEL R
Permit Number: 08457E
Effective:
09/01/2017-09/01/2019

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG734102
Exp Date: 12/07/2019

Test	g/210L	Time
DIAG	Pass	1:40pm
AIR BLK	.00	1:41pm
ACCY CHK	.07	1:41pm
AIR BLK	.00	1:42pm
SUB TEST	.00	1:43pm
AIR BLK	.00	1:44pm
SUB TEST	.00	1:45pm
AIR BLK	.00	1:46pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

TRANSYLVANIA COUNTY TRANSYLVANIA CO JAIL 870

Serial Number: 008820 Test Record Number: 1238
Test Date: 03/20/2019 Test Time: 1:47pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:47pm
FLO	Pass	1:47pm
FC	Pass	1:48pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:48pm
SRC	Pass	1:48pm
DET	Pass	1:48pm
BAR	Pass	1:48pm
BT	Pass	1:48pm

Blank Tests

Test	Status	Time
AIR	Pass	1:48pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:48pm

CRC Tests

Test	Status	Time
COMP	Pass	1:49pm
CAL	Pass	1:49pm

Preventive Maintenance
Status: Pass

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Union Instrument Location Waxhaw PD

Instrument Serial No. 008598 3620 Providence Rd, Waxhaw

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14th day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. [Signature]
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY WAXHAW PD 890

Serial Number: 008598
Test Date: 03/14/2019

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HUTCHINSON, JOSEPH E

Permit Number: 19951E

Effective:

08/01/2017-08/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG722408

Exp Date: 08/12/2019


Test	g/210L	Time
DIAG	Pass	03:06pm
AIR BLK	.00	03:07pm
ACCY CHK	.07	03:08pm
AIR BLK	.00	03:09pm
SUB TEST	.00	03:12pm
AIR BLK	.00	03:13pm
SUB TEST	.00	03:15pm
AIR BLK	.00	03:17pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

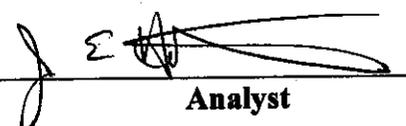

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY WAXHAW PD 890

Serial Number: 008598 Test Record Number: 796
Test Date: 03/14/2019 Test Time: 03:18pm

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	03:19pm
FLO	Pass	03:19pm
FC	Pass	03:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	03:19pm
SRC	Pass	03:19pm
DET	Pass	03:19pm
BAR	Pass	03:19pm
BT	Pass	03:19pm

Blank Tests

Test	Status	Time
AIR	Pass	03:20pm


Printer Tests

Test	Status	Time
PRNT	Pass	03:20pm

CRC Tests

Test	Status	Time
COMP	Pass	03:20pm
CAL	Pass	03:20pm

Preventive Maintenance
Status: Pass

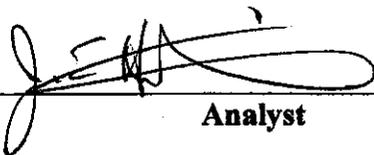

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County VANCE Instrument Location Vance Co Sheriff's Office

Instrument Serial No. 008870 156 Church St Henderson, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alex Barnes
Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

VANCE COUNTY SHERIFF'S DEPARTMENT 900

Serial Number: 008870
Test Date: 03/11/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, STOKES

Permit Number: 11434E

Effective:

05/01/2017-05/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG805801

Exp Date: 02/27/2020

Test	g/210L	Time
DIAG	Pass	11:34am
AIR BLK	.00	11:35am
ACCY CHK	.07	11:36am
AIR BLK	.00	11:37am
SUB TEST	.00	11:38am
AIR BLK	.00	11:39am
SUB TEST	.00	11:40am
AIR BLK	.00	11:41am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

VANCE COUNTY SHERIFF'S DEPARTMENT 900

Serial Number: 008870 Test Record Number: 2603
Test Date: 03/11/2019 Test Time: 11:42am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:42am
FLO	Pass	11:42am
FC	Pass	11:42am

Temperature Tests

Test	Status	Time
FC1	Pass	11:42am
SRC	Pass	11:42am
DET	Pass	11:42am
BAR	Pass	11:42am
BT	Pass	11:42am

Blank Tests

Test	Status	Time
AIR	Pass	11:43am


Printer Tests

Test	Status	Time
PRNT	Pass	11:43am

CRC Tests

Test	Status	Time
COMP	Pass	11:43am
CAL	Pass	11:43am

Preventive Maintenance
Status: Pass

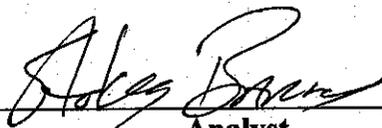

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County VANCE Instrument Location VANCE Co Sheriff's Office
Instrument Serial No. 008937 156 Church St. Henderson, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of MARCH, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alex Barnes

Signature of Certifying Official

662

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

VANCE COUNTY SHERIFF'S DEPARTMENT 900

Serial Number: 008937
Test Date: 03/11/2019

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, STOKES

Permit Number: 11434E

Effective:

05/01/2017-05/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG807102

Exp Date: 03/12/2020


Test	g/210L	Time
DIAG	Pass	11:31am
AIR BLK	.00	11:31am
ACCY CHK	.08	11:32am
AIR BLK	.00	11:33am
SUB TEST	.00	11:34am
AIR BLK	.00	11:35am
SUB TEST	.00	11:37am
AIR BLK	.00	11:38am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

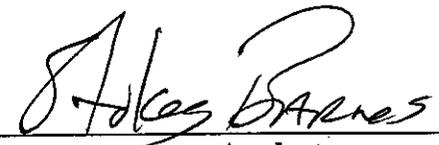

Analyst

Intox EC/IR-II: Preventive Maintenance

VANCE COUNTY SHERIFF'S DEPARTMENT 900

Serial Number: 008937 Test Record Number: 2717
Test Date: 03/11/2019 Test Time: 11:38am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:38am
FLO	Pass	11:38am
FC	Pass	11:39am

Temperature Tests

Test	Status	Time
FC1	Pass	11:39am
SRC	Pass	11:39am
DET	Pass	11:39am
BAR	Pass	11:39am
BT	Pass	11:39am

Blank Tests

Test	Status	Time
AIR	Pass	11:39am


Printer Tests

Test	Status	Time
PRNT	Pass	11:39am

CRC Tests

Test	Status	Time
COMP	Pass	11:40am
CAL	Pass	11:40am

Preventive Maintenance
Status: Pass

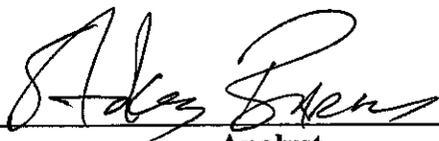

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Wake Instrument Location Raleigh PD Northeast Dist

Instrument Serial No. 008623 5228 Greens Dairy Rd Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of MARCH, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

662

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY NORTH EAST DISTRICT 910

Serial Number: 008623

Test Date: 03/08/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, STOKES

Permit Number: 11434E

Effective:

05/01/2017-05/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG716202

Exp Date: 06/11/2019

Test	g/210L	Time
DIAG	Pass	2:36pm
AIR BLK	.00	2:37pm
ACCY CHK	.08	2:37pm
AIR BLK	.00	2:39pm
SUB TEST	.00	2:39pm
AIR BLK	.00	2:40pm
SUB TEST	.00	2:41pm
AIR BLK	.00	2:42pm

Reported AC: .00 g/210L

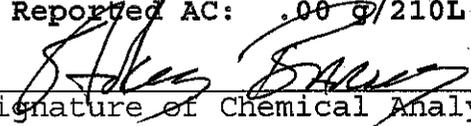
Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY NORTH EAST DISTRICT 910
Serial Number: 008623 Test Record Number: 3789
Test Date: 03/08/2019 Test Time: 2:46pm EST
System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:47pm
FLO	Pass	2:47pm
FC	Pass	2:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:47pm
SRC	Pass	2:47pm
DET	Pass	2:47pm
BAR	Pass	2:47pm
BT	Pass	2:47pm

Blank Tests

Test	Status	Time
AIR	Pass	2:48pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:48pm

CRC Tests

Test	Status	Time
COMP	Pass	2:48pm
CAL	Pass	2:48pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County WAKE Instrument Location KNIGHTDALE PD

Instrument Serial No. 008838 979 STAPLE SQUARE CT
KNIGHTDALE, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of MARCH, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY KNIGHTDALE PS 910

Serial Number: 008838
Test Date: 03/08/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, STOKES

Permit Number: 11434E

Effective:

05/01/2017-05/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG807102


Exp Date: 03/12/2020

Test	g/210L	Time
DIAG	Pass	1:37pm
AIR BLK	.00	1:37pm
ACCY CHK	.07	1:38pm
AIR BLK	.00	1:39pm
SUB TEST	.00	1:40pm
AIR BLK	.00	1:40pm
SUB TEST	.00	1:42pm
AIR BLK	.00	1:43pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

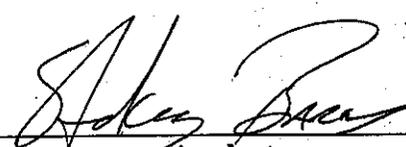
Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY KNIGHTDALE PS 910

Serial Number: 008838 Test Record Number: 1819
Test Date: 03/08/2019 Test Time: 1:43pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:44pm
FLO	Pass	1:44pm
FC	Pass	1:44pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:44pm
SRC	Pass	1:44pm
DET	Pass	1:44pm
BAR	Pass	1:44pm
BT	Pass	1:44pm

Blank Tests

Test	Status	Time
AIR	Pass	1:44pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:44pm

CRC Tests

Test	Status	Time
COMP	Pass	1:45pm
CAL	Pass	1:45pm

Preventive Maintenance
Status: Pass

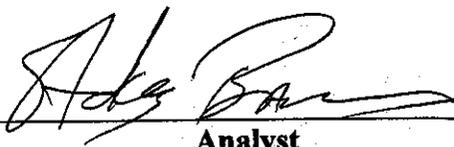

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Wake Instrument Location CARY PD

Instrument Serial No. 008587 102 Wilkinson Ave Cary, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of March, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

612
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY CARY PD 910

Serial Number: 008587
Test Date: 03/08/2019

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, STOKES

Permit Number: 11434E

Effective:

05/01/2017-05/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG734101


Exp Date: 12/07/2019

Test	g/210L	Time
DIAG	Pass	11:55am
AIR BLK	.00	11:56am
ACCY CHK	.07	11:57am
AIR BLK	.00	11:58am
SUB TEST	.00	11:59am
AIR BLK	.00	12:00pm
SUB TEST	.00	12:01pm
AIR BLK	.00	12:02pm

Reported AC: .00 g/210L

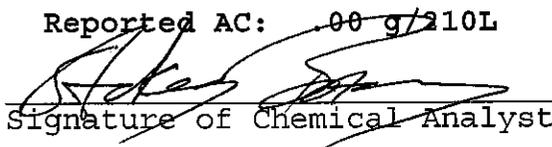
Signature of Chemical Analyst

Court CVR

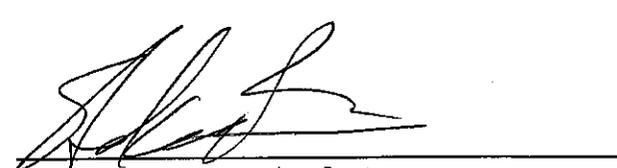
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY CARY PD 910

Serial Number: 008587 Test Record Number: 3980
Test Date: 03/08/2019 Test Time: 12:02pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:02pm
FLO	Pass	12:03pm
FC	Pass	12:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:03pm
SRC	Pass	12:03pm
DET	Pass	12:03pm
BAR	Pass	12:03pm
BT	Pass	12:03pm

Blank Tests

Test	Status	Time
AIR	Pass	12:03pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:03pm

CRC Tests

Test	Status	Time
COMP	Pass	12:04pm
CAL	Pass	12:04pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County WAKE Instrument Location APEX PD STATION 4

Instrument Serial No. 008621 1615 E. Williamson St Apex, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of MARCH, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY APEX PD

Serial Number: 008621

Test Date: 03/08/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, STOKES

Permit Number: 11434E

Effective:

05/01/2017-05/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG734101


Exp Date: 12/07/2019

Test	g/210L	Time
DIAG	Pass	10:49am
AIR BLK	.00	10:49am
ACCY CHK	.07	10:50am
AIR BLK	.00	10:51am
SUB TEST	.00	10:52am
AIR BLK	.00	10:53am
SUB TEST	.00	10:54am
AIR BLK	.00	10:55am

Reported AC: 00 g/210L


Signature of Chemical Analyst

Court CVR

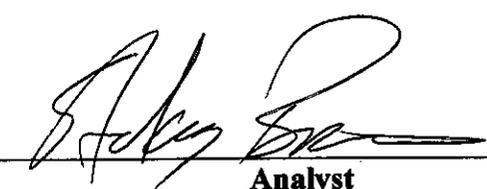
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY APEX PD

Serial Number: 008621 Test Record Number: 2599

Test Date: 03/08/2019 Test Time: 10:55am EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:56am
FLO	Pass	10:56am
FC	Pass	10:56am

Temperature Tests

Test	Status	Time
FC1	Pass	10:56am
SRC	Pass	10:56am
DET	Pass	10:56am
BAR	Pass	10:56am
BT	Pass	10:56am

Blank Tests

Test	Status	Time
AIR	Pass	10:57am

Printer Tests


Test	Status	Time
PRNT	Pass	10:57am

CRC Tests

Test	Status	Time
COMP	Pass	10:57am
CAL	Pass	10:57am

Preventive Maintenance

Status: Pass

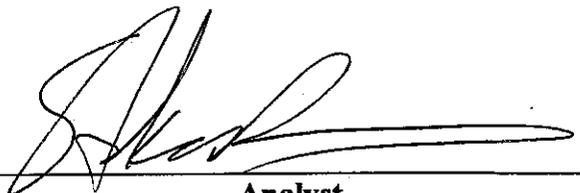

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Wake Instrument Location BAT mobile Unit 1

Instrument Serial No. 008939 Cary PD.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

660
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 1 910

Serial Number: 008939
Test Date: 03/16/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: SMITH, JASON R
Permit Number: 19145E
Effective:
03/01/2018-03/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG902201
Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	10:19pm
AIR BLK	.00	10:20pm
ACCY CHK	.08	10:21pm
AIR BLK	.00	10:21pm
SUB TEST	.00	10:22pm
AIR BLK	.00	10:23pm
SUB TEST	.00	10:25pm
AIR BLK	.00	10:26pm

Reported AC: .00 g/210L

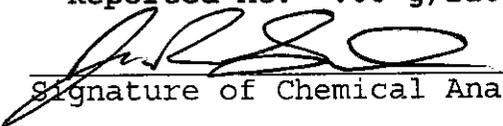
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 1 910

Serial Number: 008939 Test Record Number: 948
Test Date: 03/16/2019 Test Time: 10:29pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:29pm
FLO	Pass	10:29pm
FC	Pass	10:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:30pm
SRC	Pass	10:30pm
DET	Pass	10:30pm
BAR	Pass	10:30pm
BT	Pass	10:30pm

Blank Tests

Test	Status	Time
AIR	Pass	10:30pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:30pm

CRC Tests

Test	Status	Time
COMP	Pass	10:30pm
CAL	Pass	10:30pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Wake Instrument Location BAT Mobile Unit 1

Instrument Serial No. 008869 Lay PO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

660
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 1 910

Serial Number: 008869
Test Date: 03/16/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: SMITH, JASON R
Permit Number: 19145E
Effective:
03/01/2018-03/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG902201
Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	10:21pm
AIR BLK	.00	10:22pm
ACCY CHK	.08	10:23pm
AIR BLK	.00	10:24pm
SUB TEST	.00	10:24pm
AIR BLK	.00	10:25pm
SUB TEST	.00	10:27pm
AIR BLK	.00	10:28pm

Reported AC: .00 g/210L

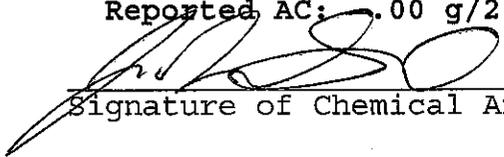

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 1 910

Serial Number: 008869 Test Record Number: 1014
Test Date: 03/16/2019 Test Time: 10:31pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:31pm
FLO	Pass	10:31pm
FC	Pass	10:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:31pm
SRC	Pass	10:31pm
DET	Pass	10:31pm
BAR	Pass	10:31pm
BT	Pass	10:31pm

Blank Tests

Test	Status	Time
AIR	Pass	10:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:32pm

CRC Tests

Test	Status	Time
COMP	Pass	10:32pm
CAL	Pass	10:32pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Wake Instrument Location Wake Co Detention Ctr

Instrument Serial No. 008612 3301 Hammond Rd Raleigh NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of MARCH, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008612
Test Date: 03/25/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, STOKES
Permit Number: 11434E
Effective:
05/01/2017-05/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG902106
Exp Date: 01/21/2021

Test	g/210L	Time
DIAG	Pass	10:52am
AIR BLK	.00	10:53am
ACCY CHK	.07	10:54am
AIR BLK	.00	10:55am
SUB TEST	.00	10:56am
AIR BLK	.00	10:57am
SUB TEST	.00	10:58am
AIR BLK	.00	10:59am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008612 Test Record Number: 4188
Test Date: 03/25/2019 Test Time: 11:00am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:00am
FLO	Pass	11:00am
FC	Pass	11:00am

Temperature Tests

Test	Status	Time
FC1	Pass	11:00am
SRC	Pass	11:00am
DET	Pass	11:00am
BAR	Pass	11:00am
BT	Pass	11:00am

Blank Tests

Test	Status	Time
AIR	Pass	11:01am

Printer Tests

Test	Status	Time
PRNT	Pass	11:01am

CRC Tests

Test	Status	Time
COMP	Pass	11:01am
CAL	Pass	11:01am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Wake Instrument Location Wake Co Detention Cor

Instrument Serial No. 008577 3301 Hammond Rd Raleigh NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of MARCH, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008577
Test Date: 03/25/2019

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, STOKES

Permit Number: 11434E

Effective:

05/01/2017-05/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG902106

Exp Date: 01/21/2021

Test	g/210L	Time
DIAG	Pass	10:45am
AIR BLK	.00	10:46am
ACCY CHK	.07	10:47am
AIR BLK	.00	10:48am
SUB TEST	.00	10:48am
AIR BLK	.00	10:49am
SUB TEST	.00	10:51am
AIR BLK	.00	10:52am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008577 Test Record Number: 4345
Test Date: 03/25/2019 Test Time: 10:53am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:53am
FLO	Pass	10:53am
FC	Pass	10:53am

Temperature Tests

Test	Status	Time
FC1	Pass	10:53am
SRC	Pass	10:53am
DET	Pass	10:53am
BAR	Pass	10:53am
BT	Pass	10:53am

Blank Tests

Test	Status	Time
AIR	Pass	10:54am

Printer Tests

Test	Status	Time
PRNT	Pass	10:54am

CRC Tests

Test	Status	Time
COMP	Pass	10:54am
CAL	Pass	10:54am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Wake Instrument Location Wake Co Detention Ctr
Instrument Serial No. 008778 3301 Hammond Rd. Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of MARCH, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alex Br...
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008778
Test Date: 03/25/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, STOKES
Permit Number: 11434E
Effective:
05/01/2017-05/01/2019

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG902106
Exp Date: 01/21/2021


Test	g/210L	Time
DIAG	Pass	10:44am
AIR BLK	.00	10:44am
ACCY CHK	.07	10:45am
AIR BLK	.00	10:47am
SUB TEST	.00	10:47am
AIR BLK	.00	10:48am
SUB TEST	.00	10:50am
AIR BLK	.00	10:51am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

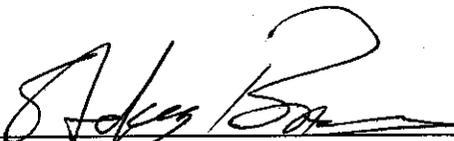

Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008778 Test Record Number: 3914
Test Date: 03/25/2019 Test Time: 10:52am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:52am
FLO	Pass	10:52am
FC	Pass	10:52am

Temperature Tests

Test	Status	Time
FC1	Pass	10:52am
SRC	Pass	10:52am
DET	Pass	10:52am
BAR	Pass	10:52am
BT	Pass	10:52am

Blank Tests

Test	Status	Time
AIR	Pass	10:53am


Printer Tests

Test	Status	Time
PRNT	Pass	10:53am

CRC Tests

Test	Status	Time
COMP	Pass	10:53am
CAL	Pass	10:53am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Wake

Instrument Location Wake Co. Detention CTR

Instrument Serial No. 008760

3301 HAMMOND RD RALEIGH, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of MARCH, 2019, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008760
Test Date: 03/25/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, STOKES

Permit Number: 11434E

Effective:

05/01/2017-05/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG902106

Exp Date: 01/21/2021


Test	g/210L	Time
DIAG	Pass	10:38am
AIR BLK	.00	10:39am
ACCY CHK	.08	10:39am
AIR BLK	.00	10:40am
SUB TEST	.00	10:41am
AIR BLK	.00	10:42am
SUB TEST	.00	10:44am
AIR BLK	.00	10:45am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

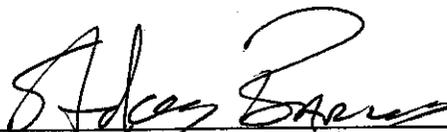

Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008760 Test Record Number: 3306
Test Date: 03/25/2019 Test Time: 10:46am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:46am
FLO	Pass	10:46am
FC	Pass	10:46am

Temperature Tests

Test	Status	Time
FC1	Pass	10:46am
SRC	Pass	10:46am
DET	Pass	10:46am
BAR	Pass	10:46am
BT	Pass	10:46am

Blank Tests

Test	Status	Time
AIR	Pass	10:47am


Printer Tests

Test	Status	Time
PRNT	Pass	10:47am

CRC Tests

Test	Status	Time
COMP	Pass	10:47am
CAL	Pass	10:47am

Preventive Maintenance
Status: Pass

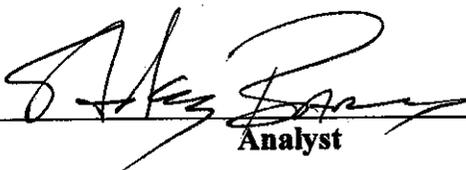

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Washington Instrument Location Washington Co. S.O.
Instrument Serial No. 008829 Adams St., Plymouth, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Key

Signature of Certifying Official

643

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WASHINGTON COUNTY SHERIFF'S OFFICE 930

Serial Number: 008829
Test Date: 03/29/2019

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GUARD, KELLY G

Permit Number: 12955E

Effective:

06/01/2017-06/01/2019

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG902201

Exp Date: 01/22/2021


Test	g/210L	Time
DIAG	Pass	9:40am
AIR BLK	.00	9:41am
ACCY CHK	.07	9:42am
AIR BLK	.00	9:43am
SUB TEST	.00	9:43am
AIR BLK	.00	9:44am
SUB TEST	.00	9:46am
AIR BLK	.00	9:47am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WASHINGTON COUNTY SHERIFF'S OFFICE 930

Serial Number: 008829 Test Record Number: 898
Test Date: 03/29/2019 Test Time: 9:49am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:49am
FLO	Pass	9:49am
FC	Pass	9:50am

Temperature Tests

Test	Status	Time
FC1	Pass	9:50am
SRC	Pass	9:50am
DET	Pass	9:50am
BAR	Pass	9:50am
BT	Pass	9:50am

Blank Tests

Test	Status	Time
AIR	Pass	9:50am


Printer Tests

Test	Status	Time
PRNT	Pass	9:50am

CRC Tests

Test	Status	Time
COMP	Pass	9:51am
CAL	Pass	9:51am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Wilson

Instrument Location BAT Mobile Unit 1


Instrument Serial No. 008869

Wilson PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of March, 2019 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

660
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

WILSON COUNTY BAT MOBILE UNIT 1 970

Serial Number: 008869 Test Record Number: 1009
Test Date: 03/14/2019 Test Time: 10:30pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:30pm
FLO	Pass	10:30pm
FC	Pass	10:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:30pm
SRC	Pass	10:30pm
DET	Pass	10:30pm
BAR	Pass	10:30pm
BT	Pass	10:30pm

Blank Tests

Test	Status	Time
AIR	Pass	10:31pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:31pm

CRC Tests

Test	Status	Time
COMP	Pass	10:31pm
CAL	Pass	10:31pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

WILSON COUNTY BAT MOBILE UNIT 1 970

Serial Number: 008869
Test Date: 03/14/2019

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: SMITH, JASON R
Permit Number: 19145E
Effective:
03/01/2018-03/01/2020

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG902201
Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	10:21pm
AIR BLK	.00	10:22pm
ACCY CHK	.08	10:22pm
AIR BLK	.00	10:23pm
SUB TEST	.00	10:24pm
AIR BLK	.00	10:25pm
SUB TEST	.00	10:27pm
AIR BLK	.00	10:28pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**