DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County ALAMANCE Instrument Location ALAMANCE CO JAIL

Instrument Serial No. 008853 109 S. MAPLE ST GRAHAM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of MARCH, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA
MAY 20, 1775
APRIL 12, 1776
ESSE QUAM VIDERI

Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: *008853*
Test Date: *03/10/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, STOKES*
Permit Number: *11434E*
Effective:
04/01/2019-04/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919902
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	11:14am
AIR BLK	.00	11:15am
ACCY CHK	.08	11:16am
AIR BLK	.00	11:17am
SUB TEST	**.00**	**11:18am**
AIR BLK	.00	11:19am
SUB TEST	**.00**	**11:20am**
AIR BLK	.00	11:21am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: *008853* Test Record Number: *3045*
Test Date: *03/10/2020* Test Time: *11:22am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:22am
FLO	Pass	11:22am
FC	Pass	11:22am

Temperature Tests

Test	Status	Time
FC1	Pass	11:22am
SRC	Pass	11:22am
DET	Pass	11:22am
BAR	Pass	11:22am
BT	Pass	11:22am

Blank Tests

Test	Status	Time
AIR	Pass	11:23am

Printer Tests

Test	Status	Time
PRNT	Pass	11:23am

CRC Tests

Test	Status	Time
COMP	Pass	11:23am
CAL	Pass	11:23am

Preventive Maintenance
Status: Pass

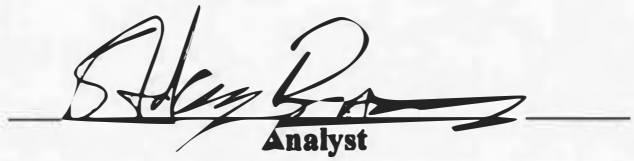

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County ALAMANCE Instrument Location ALAMANCE CO. JAIL

Instrument Serial No. 008913 109 S. MAPLE ST. GRAHAM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 06 day of MARCH, 20 20 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

R L D Smith
Signature of Certifying Official

637
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: *008913*
Test Date: *03/06/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Smith, Brian D*
Permit Number: *0032-6608*
Effective:
07/09/2019-07/09/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919902
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	2:37pm
AIR BLK	.00	2:38pm
ACCY CHK	.08	2:39pm
AIR BLK	.00	2:40pm
SUB TEST	**.00**	**2:40pm**
AIR BLK	.00	2:42pm
SUB TEST	**.00**	**2:43pm**
AIR BLK	.00	2:44pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: *008913* Test Record Number: *3825*
Test Date: *03/06/2020* Test Time: *2:44pm EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:45pm
FLO	Pass	2:45pm
FC	Pass	2:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:45pm
SRC	Pass	2:45pm
DET	Pass	2:45pm
BAR	Pass	2:45pm
BT	Pass	2:45pm

Blank Tests

Test	Status	Time
AIR	Pass	2:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:46pm

CRC Tests

Test	Status	Time
COMP	Pass	2:46pm
CAL	Pass	2:46pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Alleghany Instrument Location Alleghany Co Jail

Instrument Serial No. 008890 Sparta, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALLEGHANY COUNTY ALLEGHANY CO JAIL 020

Serial Number: *008890*
Test Date: *03/27/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BURNETTE, ANTHONY J*
Permit Number: *11304E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG821801
Exp Date: 08/06/2020

Test	g/210L	Time
DIAG	Pass	1:21pm
AIR BLK	.00	1:22pm
ACCY CHK	.07	1:23pm
AIR BLK	.00	1:23pm
SUB TEST	**.00**	**1:24pm**
AIR BLK	.00	1:25pm
SUB TEST	**.00**	**1:26pm**
AIR BLK	.00	1:27pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ALLEGHANY COUNTY ALLEGHANY CO JAIL 020

Serial Number: *008890* Test Record Number: *801*
Test Date: *03/27/2020* Test Time: *1:28pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:28pm
FLO	Pass	1:28pm
FC	Pass	1:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:29pm
SRC	Pass	1:29pm
DET	Pass	1:29pm
BAR	Pass	1:29pm
BT	Pass	1:29pm

Blank Tests

Test	Status	Time
AIR	Pass	1:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:29pm

CRC Tests

Test	Status	Time
COMP	Pass	1:29pm
CAL	Pass	1:29pm

Preventive Maintenance
Status: Pass

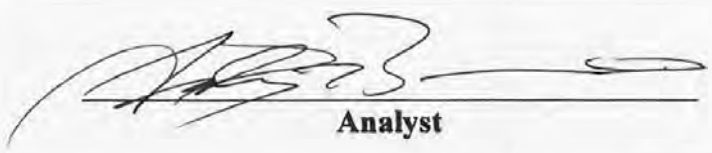

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Alexander Co. Instrument Location Alexander Co. Sheriff's Office

Instrument Serial No. EC8591 Wadesboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th **day of** March, 2020, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

ANSON COUNTY SHERIFF'S OFFICE 030

Serial Number: *008597*
Test Date: *03/25/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG902202
Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	4:31pm
AIR BLK	.00	4:31pm
ACCY CHK	.08	4:32pm
AIR BLK	.00	4:33pm
SUB TEST	**.00**	**4:34pm**
AIR BLK	.00	4:35pm
SUB TEST	**.00**	**4:36pm**
AIR BLK	.00	4:37pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ANSON COUNTY SHERIFF'S OFFICE 030

Serial Number: *008597* Test Record Number: *1742*
Test Date: *03/25/2020* Test Time: *4:38pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:38pm
FLO	Pass	4:38pm
FC	Pass	4:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:38pm
SRC	Pass	4:38pm
DET	Pass	4:38pm
BAR	Pass	4:38pm
BT	Pass	4:38pm

Blank Tests

Test	Status	Time
AIR	Pass	4:39pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:39pm

CRC Tests

Test	Status	Time
COMP	Pass	4:39pm
CAL	Pass	4:39pm

Preventive Maintenance
Status: Pass

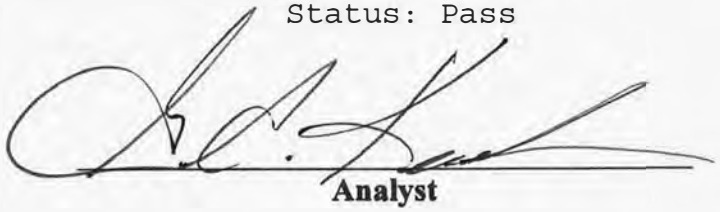

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Anson Co. Instrument Location Anson Co. Sheriff's Office

Instrument Serial No. 008139 Wadesboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th **day of** March **, 20**20**, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

ANSON COUNTY SHERIFF'S OFFICE 030

Serial Number: *008739*
Test Date: *03/25/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG902202
Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	4:32pm
AIR BLK	.00	4:33pm
ACCY CHK	.08	4:34pm
AIR BLK	.00	4:35pm
SUB TEST	**.00**	**4:36pm**
AIR BLK	.00	4:37pm
SUB TEST	**.00**	**4:38pm**
AIR BLK	.00	4:39pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ANSON COUNTY SHERIFF'S OFFICE 030

Serial Number: *008739* Test Record Number: *516*
Test Date: *03/25/2020* Test Time: *4:40pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:41pm
FLO	Pass	4:41pm
FC	Pass	4:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:41pm
SRC	Pass	4:41pm
DET	Pass	4:41pm
BAR	Pass	4:41pm
BT	Pass	4:41pm

Blank Tests

Test	Status	Time
AIR	Pass	4:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:41pm

CRC Tests

Test	Status	Time
COMP	Pass	4:42pm
CAL	Pass	4:42pm

Preventive Maintenance Status: Pass

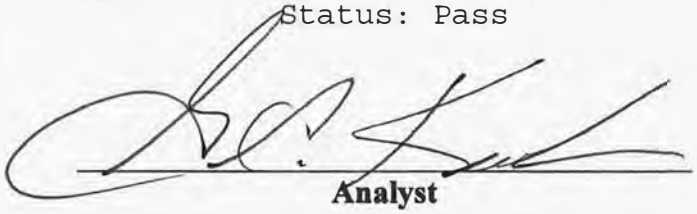

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Beaufort Instrument Location Belhaven P.D

Instrument Serial No. 008928 Belhaven, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th **day of** March, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA MAY 20, 1775 APRIL 12, 1776 ESSE QUAM VIDERI

Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BEAUFORT COUNTY BELHAVEN PD 060

Serial Number: *008928*
Test Date: *03/19/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *GUARD, KELLY G*
Permit Number: *12955E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG902201
Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	12:09pm
AIR BLK	.00	12:09pm
ACCY CHK	.08	12:10pm
AIR BLK	.00	12:11pm
SUB TEST	**.00**	**12:12pm**
AIR BLK	.00	12:12pm
SUB TEST	**.00**	**12:14pm**
AIR BLK	.00	12:15pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BEAUFORT COUNTY BELHAVEN PD 060

Serial Number: *008928* Test Record Number: *412*
Test Date: *03/19/2020* Test Time: *12:17pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:18pm
FLO	Pass	12:18pm
FC	Pass	12:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:18pm
SRC	Pass	12:18pm
DET	Pass	12:18pm
BAR	Pass	12:18pm
BT	Pass	12:18pm

Blank Tests

Test	Status	Time
AIR	Pass	12:18pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:18pm

CRC Tests

Test	Status	Time
COMP	Pass	12:19pm
CAL	Pass	12:19pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County BLADEN Instrument Location BLADEN COUNTY

Instrument Serial No. 008818 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 **day of** MARCH **, 20** 20**, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Alan Ray Bass — Signature of Certifying Official

648 — Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BLADEN COUNTY DETENTION CENTER 080

Serial Number: *008818*
Test Date: *03/20/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, ALVIN R*
Permit Number: *15671E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911506
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	1:20pm
AIR BLK	.00	1:21pm
ACCY CHK	.08	1:22pm
AIR BLK	.00	1:23pm
SUB TEST	**.00**	**1:24pm**
AIR BLK	.00	1:24pm
SUB TEST	**.00**	**1:26pm**
AIR BLK	.00	1:27pm

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

Alvin Ray Barnes
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BLADEN COUNTY DETENTION CENTER 080

Serial Number: *008818* Test Record Number: *1603*
Test Date: *03/20/2020* Test Time: *1:28pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:28pm
FLO	Pass	1:28pm
FC	Pass	1:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:29pm
SRC	Pass	1:29pm
DET	Pass	1:29pm
BAR	Pass	1:29pm
BT	Pass	1:29pm

Blank Tests

Test	Status	Time
AIR	Pass	1:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:29pm

CRC Tests

Test	Status	Time
COMP	Pass	1:30pm
CAL	Pass	1:30pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County BLADEN Instrument Location BLADEN COUNTY

Instrument Serial No. 008894 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 **day of** MARCH **, 20** 20**, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

BLADEN COUNTY DETENTION CENTER 080

Serial Number: *008894*
Test Date: *03/20/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, ALVIN R*
Permit Number: *15671E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911501
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	1:21pm
AIR BLK	.00	1:22pm
ACCY CHK	.08	1:23pm
AIR BLK	.00	1:24pm
SUB TEST	**.00**	**1:25pm**
AIR BLK	.00	1:25pm
SUB TEST	**.00**	**1:27pm**
AIR BLK	.00	1:28pm

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

Alvin Ray Barnes
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BLADEN COUNTY DETENTION CENTER 080

Serial Number: *008894* Test Record Number: *1217*
Test Date: *03/20/2020* Test Time: *1:28pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:29pm
FLO	Pass	1:29pm
FC	Pass	1:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:29pm
SRC	Pass	1:29pm
DET	Pass	1:29pm
BAR	Pass	1:29pm
BT	Pass	1:29pm

Blank Tests

Test	Status	Time
AIR	Pass	1:30pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:30pm

CRC Tests

Test	Status	Time
COMP	Pass	1:30pm
CAL	Pass	1:30pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Burke Instrument Location Burke Co Jail

Instrument Serial No. 008831 Morganton NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 day of March, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

658
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

BURKE COUNTY BURKE-CATAWBA JAIL 110

Serial Number: *008831*
Test Date: *03/30/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *TOWERY, CHAD V*
Permit Number: *26632E*
Effective:
05/01/2019-05/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919902
Exp Date: 07/28/2021

Test	g/210L	Time
DIAG	Pass	8:53am
AIR BLK	.00	8:54am
ACCY CHK	.08	8:54am
AIR BLK	.00	8:55am
SUB TEST	**.00**	**8:56am**
AIR BLK	.00	8:57am
SUB TEST	**.00**	**8:58am**
AIR BLK	.00	8:59am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BURKE COUNTY BURKE-CATAWBA JAIL 110

Serial Number: *008831* Test Record Number: *2222*
Test Date: *03/30/2020* Test Time: *9:00am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:01am
FLO	Pass	9:01am
FC	Pass	9:01am

Temperature Tests

Test	Status	Time
FC1	Pass	9:01am
SRC	Pass	9:01am
DET	Pass	9:01am
BAR	Pass	9:01am
BT	Pass	9:01am

Blank Tests

Test	Status	Time
AIR	Pass	9:02am

Printer Tests

Test	Status	Time
PRNT	Pass	9:02am

CRC Tests

Test	Status	Time
COMP	Pass	9:02am
CAL	Pass	9:02am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Burke Instrument Location Burke Co Jail

Instrument Serial No. 006904 Morganton NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 day of March, 20 20 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

658
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

BURKE COUNTY BURKE-CATAWBA JAIL 110

Serial Number: *008904*
Test Date: *03/30/2020*

Citation Number: *M0000000-0*
Subject's Name:
PRVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *TOWERY, CHAD V*
Permit Number: *26632E*
Effective:
05/01/2019-05/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG920301
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	8:48am
AIR BLK	.00	8:49am
ACCY CHK	.08	8:49am
AIR BLK	.00	8:50am
SUB TEST	**.00**	**8:51am**
AIR BLK	.00	8:52am
SUB TEST	**.00**	**8:54am**
AIR BLK	.00	8:54am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BURKE COUNTY BURKE-CATAWBA JAIL 110

Serial Number: *008904* Test Record Number: *2474*
Test Date: *03/30/2020* Test Time: *8:55am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:56am
FLO	Pass	8:56am
FC	Pass	8:56am

Temperature Tests

Test	Status	Time
FC1	Pass	8:56am
SRC	Pass	8:56am
DET	Pass	8:56am
BAR	Pass	8:56am
BT	Pass	8:56am

Blank Tests

Test	Status	Time
AIR	Pass	8:57am

Printer Tests

Test	Status	Time
PRNT	Pass	8:57am

CRC Tests

Test	Status	Time
COMP	Pass	8:57am
CAL	Pass	8:57am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Buncombe Instrument Location Black Mobile Unit 2

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of March, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

658
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 02 100

Serial Number: *008970*
Test Date: *03/17/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *TOWERY, CHAD V*
Permit Number: *26632E*
Effective:
05/01/2019-05/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG902201
Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	8:52pm
AIR BLK	.00	8:53pm
ACCY CHK	.08	8:54pm
AIR BLK	.00	8:54pm
SUB TEST	**.00**	**8:55pm**
AIR BLK	.00	8:56pm
SUB TEST	**.00**	**8:57pm**
AIR BLK	.00	8:58pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 02 100

Serial Number: *008970* Test Record Number: *720*
Test Date: *03/17/2020* Test Time: *8:59pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:59pm
FLO	Pass	8:59pm
FC	Pass	9:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:00pm
SRC	Pass	9:00pm
DET	Pass	9:00pm
BAR	Pass	9:00pm
BT	Pass	9:00pm

Blank Tests

Test	Status	Time
AIR	Pass	9:00pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:00pm

CRC Tests

Test	Status	Time
COMP	Pass	9:01pm
CAL	Pass	9:01pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Cabarrus Instrument Location Cabarrus County SO

Instrument Serial No. 008590 30 Corban Ave, Concord

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of March, 20 20 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: *008590*
Test Date: *03/04/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Hays, Mark D*
Permit Number: *0011-3099*
Effective:
11/13/2019-11/13/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG920301
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	12:36pm
AIR BLK	.00	12:37pm
ACCY CHK	.08	12:38pm
AIR BLK	.00	12:39pm
SUB TEST	**.00**	**12:40pm**
AIR BLK	.00	12:41pm
SUB TEST	**.00**	**12:43pm**
AIR BLK	.00	12:43pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: *008590* Test Record Number: *3413*
Test Date: *03/04/2020* Test Time: *12:45pm EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:45pm
FLO	Pass	12:45pm
FC	Pass	12:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:46pm
SRC	Pass	12:46pm
DET	Pass	12:46pm
BAR	Pass	12:46pm
BT	Pass	12:46pm

Blank Tests

Test	Status	Time
AIR	Pass	12:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:46pm

CRC Tests

Test	Status	Time
COMP	Pass	12:47pm
CAL	Pass	12:47pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Cabarrus Instrument Location Cabarrus County SO

Instrument Serial No. 008792 30 Corban Ave, Concord

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of March, 20 20 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: *008792*
Test Date: *03/04/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Hays, Mark D*
Permit Number: *0011-3099*
Effective:
11/13/2019-11/13/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919901
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	1:02pm
AIR BLK	.00	1:03pm
ACCY CHK	.08	1:04pm
AIR BLK	.00	1:05pm
SUB TEST	**.00**	**1:06pm**
AIR BLK	.00	1:07pm
SUB TEST	**.00**	**1:08pm**
AIR BLK	.00	1:09pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: *008792* Test Record Number: *3048*
Test Date: *03/04/2020* Test Time: *1:10pm EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:11pm
FLO	Pass	1:11pm
FC	Pass	1:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:11pm
SRC	Pass	1:11pm
DET	Pass	1:11pm
BAR	Pass	1:11pm
BT	Pass	1:11pm

Blank Tests

Test	Status	Time
AIR	Pass	1:11pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:11pm

CRC Tests

Test	Status	Time
COMP	Pass	1:12pm
CAL	Pass	1:12pm

Preventive Maintenance
Status: Pass

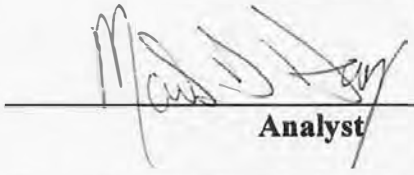

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Camden Instrument Location Camden Co. S.O.

Instrument Serial No. 008940 113 Hwy 343, Camden, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24th **day of** MARCH, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CAMDEN COUNTY CAMDEN CC SO 140

Serial Number: *008940*
Test Date: *03/20/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Linda A*
Permit Number: *0045-5468*
Effective:
07/08/2019-07/08/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911501
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	11:56am
AIR BLK	.00	11:56am
ACCY CHK	.08	11:57am
AIR BLK	.00	11:58am
SUB TEST	**.00**	**11:59am**
AIR BLK	.00	12:00pm
SUB TEST	**.00**	**12:01pm**
AIR BLK	.00	12:02pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Linda A. Keesler
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CAMDEN COUNTY CAMDEN CO SO 140

Serial Number: *008940* Test Record Number: *1010*
Test Date: *03/20/2020* Test Time: *12:03pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:04pm
FLO	Pass	12:04pm
FC	Pass	12:04pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:04pm
SRC	Pass	12:04pm
DET	Pass	12:04pm
BAR	Pass	12:04pm
BT	Pass	12:04pm

Blank Tests

Test	Status	Time
AIR	Pass	12:04pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:04pm

CRC Tests

Test	Status	Time
COMP	Pass	12:05pm
CAL	Pass	12:05pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County CARTERET Instrument Location CARTERET COUNTY DETENTION CENTER

Instrument Serial No. 008605

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 **day of** MARCH, **20** 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Alan Ray Bass — Signature of Certifying Official

C48 — Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY DETENTION CENTER 150

Serial Number: *008605*
Test Date: *03/23/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, ALVIN R*
Permit Number: *15671E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG934001
Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	1:12pm
AIR BLK	.00	1:13pm
ACCY CHK	.07	1:14pm
AIR BLK	.00	1:15pm
SUB TEST	**.00**	**1:15pm**
AIR BLK	.00	1:16pm
SUB TEST	**.00**	**1:18pm**
AIR BLK	.00	1:19pm

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY DETENTION CENTER 150

Serial Number: *008605* Test Record Number: *3943*
Test Date: *03/23/2020* Test Time: *1:19pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:19pm
FLO	Pass	1:19pm
FC	Pass	1:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:20pm
SRC	Pass	1:20pm
DET	Pass	1:20pm
BAR	Pass	1:20pm
BT	Pass	1:20pm

Blank Tests

Test	Status	Time
AIR	Pass	1:20pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:20pm

CRC Tests

Test	Status	Time
COMP	Pass	1:21pm
CAL	Pass	1:21pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County CARTERET Instrument Location EMERALD ISLE

Instrument Serial No. 008620 POLICE DEPT.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of MARCH, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

CARTERET COUNTY EMERALD ISLE PD 150

Serial Number: *008620*
Test Date: *03/23/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, ALVIN R*
Permit Number: *15671E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919901
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	10:17am
AIR BLK	.00	10:17am
ACCY CHK	.08	10:18am
AIR BLK	.00	10:19am
SUB TEST	**.00**	**10:20am**
AIR BLK	.00	10:21am
SUB TEST	**.00**	**10:22am**
AIR BLK	.00	10:23am

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY EMERALD ISLE PD 150

Serial Number: *008620* Test Record Number: *2084*
Test Date: *03/23/2020* Test Time: *10:24am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:24am
FLO	Pass	10:24am
FC	Pass	10:24am

Temperature Tests

Test	Status	Time
FC1	Pass	10:24am
SRC	Pass	10:24am
DET	Pass	10:24am
BAR	Pass	10:24am
BT	Pass	10:24am

Blank Tests

Test	Status	Time
AIR	Pass	10:25am

Printer Tests

Test	Status	Time
PRNT	Pass	10:25am

CRC Tests

Test	Status	Time
COMP	Pass	10:25am
CAL	Pass	10:25am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County CARTERET Instrument Location MOREHEAD CITY POLICE DEPT

Instrument Serial No. 008731

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 **day of** MARCH, **20** 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is ~~functioning~~ properly.**

Alan Ray Barnes
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

CARTERET COUNTY MOREHEAD CITY PD 150

Serial Number: *008731*
Test Date: *03/23/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, ALVIN R*
Permit Number: *15671E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911501
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	12:17pm
AIR BLK	.00	12:18pm
ACCY CHK	.08	12:18pm
AIR BLK	.00	12:19pm
SUB TEST	**.00**	**12:20pm**
AIR BLK	.00	12:21pm
SUB TEST	**.00**	**12:22pm**
AIR BLK	.00	12:23pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Alvin Ray Barnes

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY MOREHEAD CITY PD 150

Serial Number: *008731* Test Record Number: *2219*
Test Date: *03/23/2020* Test Time: *12:24pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:24pm
FLO	Pass	12:24pm
FC	Pass	12:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:25pm
SRC	Pass	12:25pm
DET	Pass	12:25pm
BAR	Pass	12:25pm
BT	Pass	12:25pm

Blank Tests

Test	Status	Time
AIR	Pass	12:25pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:25pm

CRC Tests

Test	Status	Time
COMP	Pass	12:25pm
CAL	Pass	12:25pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County CARTERET Instrument Location ATLANTIC BEACH POLICE DEPT

Instrument Serial No. 008785

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of MARCH, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

CARTERET COUNTY ATLANTIC BEACH PD 150

Serial Number: *008785*
Test Date: *03/23/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, ALVIN R*
Permit Number: *15671E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG934001
Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	11:40am
AIR BLK	.00	11:41am
ACCY CHK	.08	11:42am
AIR BLK	.00	11:43am
SUB TEST	**.00**	**11:44am**
AIR BLK	.00	11:45am
SUB TEST	**.00**	**11:46am**
AIR BLK	.00	11:47am

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

_____
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY ATLANTIC BEACH PD 150

Serial Number: *008785* Test Record Number: *1204*
Test Date: *03/23/2020* Test Time: *11:47am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:48am
FLO	Pass	11:48am
FC	Pass	11:48am

Temperature Tests

Test	Status	Time
FC1	Pass	11:48am
SRC	Pass	11:48am
DET	Pass	11:48am
BAR	Pass	11:48am
BT	Pass	11:48am

Blank Tests

Test	Status	Time
AIR	Pass	11:48am

Printer Tests

Test	Status	Time
PRNT	Pass	11:48am

CRC Tests

Test	Status	Time
COMP	Pass	11:49am
CAL	Pass	11:49am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County CARTERET Instrument Location CARTERET COUNTY

Instrument Serial No. 00E882 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 **day of** MARCH, **20** 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

CARTERET COUNTY DETENTION CENTER 150

Serial Number: *008882*
Test Date: *03/23/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, ALVIN R*
Permit Number: *15671E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919901
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	1:13pm
AIR BLK	.00	1:13pm
ACCY CHK	.08	1:14pm
AIR BLK	.00	1:15pm
SUB TEST	**.00**	**1:16pm**
AIR BLK	.00	1:16pm
SUB TEST	**.00**	**1:18pm**
AIR BLK	.00	1:19pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY DETENTION CENTER 150

Serial Number: *008882* Test Record Number: *1950*
Test Date: *03/23/2020* Test Time: *1:19pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:20pm
FLO	Pass	1:20pm
FC	Pass	1:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:20pm
SRC	Pass	1:20pm
DET	Pass	1:20pm
BAR	Pass	1:20pm
BT	Pass	1:20pm

Blank Tests

Test	Status	Time
AIR	Pass	1:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:21pm

CRC Tests

Test	Status	Time
COMP	Pass	1:21pm
CAL	Pass	1:21pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Catawba Instrument Location Catawba County SO

Instrument Serial No. 008821 100 B Southwest Blvd, Newton

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th **day of** March, **20**20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Joseph E. Hudd
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: *008821*
Test Date: *03/30/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Hutchinson, Joseph E*
Permit Number: *0035-6075*
Effective:
07/09/2019-07/09/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG814901
Exp Date: 05/29/2020

Test	g/210L	Time
DIAG	Pass	2:24pm
AIR BLK	.00	2:25pm
ACCY CHK	.07	2:25pm
AIR BLK	.00	2:26pm
SUB TEST	**.00**	**2:27pm**
AIR BLK	.00	2:28pm
SUB TEST	**.00**	**2:29pm**
AIR BLK	.00	2:31pm

Reported AC: .00 g/210L

J. E. Hutchinson
Signature of Chemical Analyst

Court CVR

J. E. Hutchinson
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: *008821* Test Record Number: *2072*
Test Date: *03/30/2020* Test Time: *2:32pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:32pm
FLO	Pass	2:32pm
FC	Pass	2:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:32pm
SRC	Pass	2:32pm
DET	Pass	2:32pm
BAR	Pass	2:32pm
BT	Pass	2:32pm

Blank Tests

Test	Status	Time
AIR	Pass	2:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:33pm

CRC Tests

Test	Status	Time
COMP	Pass	2:33pm
CAL	Pass	2:33pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Catawba Instrument Location Catawba County SO

Instrument Serial No. 008821 100 B Southwest Blvd, Newton

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th **day of** March, **20**20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Joseph E. Hudd
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: *008821*
Test Date: *03/30/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Hutchinson, Joseph E*
Permit Number: *0035-6075*
Effective:
07/09/2019-07/09/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG814901
Exp Date: 05/29/2020

Test	g/210L	Time
DIAG	Pass	2:24pm
AIR BLK	.00	2:25pm
ACCY CHK	.07	2:25pm
AIR BLK	.00	2:26pm
SUB TEST	**.00**	**2:27pm**
AIR BLK	.00	2:28pm
SUB TEST	**.00**	**2:29pm**
AIR BLK	.00	2:31pm

Reported AC: .00 g/210L

J. E. Hutchinson
Signature of Chemical Analyst

Court CVR

J. E. Hutchinson
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: *008821* Test Record Number: *2072*
Test Date: *03/30/2020* Test Time: *2:32pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:32pm
FLO	Pass	2:32pm
FC	Pass	2:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:32pm
SRC	Pass	2:32pm
DET	Pass	2:32pm
BAR	Pass	2:32pm
BT	Pass	2:32pm

Blank Tests

Test	Status	Time
AIR	Pass	2:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:33pm

CRC Tests

Test	Status	Time
COMP	Pass	2:33pm
CAL	Pass	2:33pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Cherokee Instrument Location Cherokee Co. Jail

Instrument Serial No. 008622 Murphy, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of March, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

David R Cathey — Signature of Certifying Official

635 — Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHEROKEE COUNTY CHEROKEE COUNTY JAIL
190

Serial Number: *008622*
Test Date: *03/12/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
07/12/2019-07/12/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG920301
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	11:09am
AIR BLK	.00	11:10am
ACCY CHK	.08	11:11am
AIR BLK	.00	11:12am
SUB TEST	**.00**	**11:13am**
AIR BLK	.00	11:13am
SUB TEST	**.00**	**11:15am**
AIR BLK	.00	11:16am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CHEROKEE COUNTY CHEROKEE COUNTY JAIL 190

Serial Number: *008622* Test Record Number: *1117*
Test Date: *03/12/2020* Test Time: *11:18am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:18am
FLO	Pass	11:18am
FC	Pass	11:18am

Temperature Tests

Test	Status	Time
FC1	Pass	11:19am
SRC	Pass	11:19am
DET	Pass	11:19am
BAR	Pass	11:19am
BT	Pass	11:19am

Blank Tests

Test	Status	Time
AIR	Pass	11:19am

Printer Tests

Test	Status	Time
PRNT	Pass	11:19am

CRC Tests

Test	Status	Time
COMP	Pass	11:19am
CAL	Pass	11:19am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Cherokee Instrument Location Cherokee Co. Jail

Instrument Serial No. 008711 Murphy, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

David R. Cutler
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHEROKEE COUNTY CHEROKEE COUNTY JAIL
190

Serial Number: *008711*
Test Date: *03/12/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
07/12/2019-07/12/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911506
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	11:07am
AIR BLK	.00	11:08am
ACCY CHK	.07	11:09am
AIR BLK	.00	11:10am
SUB TEST	**.00**	**11:11am**
AIR BLK	.00	11:12am
SUB TEST	**.00**	**11:13am**
AIR BLK	.00	11:14am

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CHEROKEE COUNTY CHEROKEE COUNTY JAIL 190

Serial Number: *008711* Test Record Number: *1059*
Test Date: *03/12/2020* Test Time: *11:16am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:17am
FLO	Pass	11:17am
FC	Pass	11:17am

Temperature Tests

Test	Status	Time
FC1	Pass	11:17am
SRC	Pass	11:17am
DET	Pass	11:17am
BAR	Pass	11:17am
BT	Pass	11:17am

Blank Tests

Test	Status	Time
AIR	Pass	11:17am

Printer Tests

Test	Status	Time
PRNT	Pass	11:18am

CRC Tests

Test	Status	Time
COMP	Pass	11:18am
CAL	Pass	11:18am

Preventive Maintenance
Status: Pass

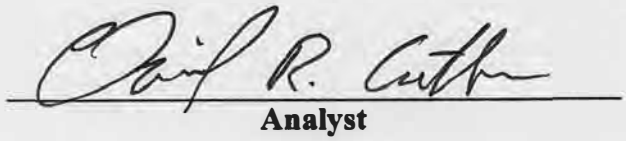

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Clay Instrument Location Clay Co. Jail

Instrument Serial No. 008608 Hayesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLAY COUNTY CLAY COUNTY JAIL 210

Serial Number: *008608*
Test Date: *03/10/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
07/12/2019-07/12/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG902106
Exp Date: 01/21/2021

Test	g/210L	Time
DIAG	Pass	10:22am
AIR BLK	.00	10:23am
ACCY CHK	.08	10:24am
AIR BLK	.00	10:25am
SUB TEST	**.00**	**10:26am**
AIR BLK	.00	10:26am
SUB TEST	**.00**	**10:28am**
AIR BLK	.00	10:29am

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

Daniel R. Cutler
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CLAY COUNTY CLAY COUNTY JAIL 210

Serial Number: *008608* Test Record Number: *1287*
Test Date: *03/10/2020* Test Time: *10:30am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:30am
FLO	Pass	10:30am
FC	Pass	10:30am

Temperature Tests

Test	Status	Time
FC1	Pass	10:31am
SRC	Pass	10:31am
DET	Pass	10:31am
BAR	Pass	10:31am
BT	Pass	10:31am

Blank Tests

Test	Status	Time
AIR	Pass	10:31am

Printer Tests

Test	Status	Time
PRNT	Pass	10:31am

CRC Tests

Test	Status	Time
COMP	Pass	10:31am
CAL	Pass	10:31am

Preventive Maintenance
Status: Pass

David R. Cuthbert

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Cleveland Instrument Location Cleveland County SO

Instrument Serial No. 008867 Annex

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 **day of** March, 2020, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

CLEVELAND COUNTY CLEVELAND SO-ANNEX 220

Serial Number: *008887*
Test Date: *03/30/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Hays, Mark D*
Permit Number: *0011-3099*
Effective:
11/13/2019-11/13/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG933901
Exp Date: 12/05/2021

Test	g/210L	Time
DIAG	Pass	11:26am
AIR BLK	.00	11:27am
ACCY CHK	.08	11:27am
AIR BLK	.00	11:29am
SUB TEST	**.00**	**11:30am**
AIR BLK	.00	11:30am
SUB TEST	**.00**	**11:32am**
AIR BLK	.00	11:33am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CLEVELAND COUNTY CLEVELAND SO-ANNEX 220

Serial Number: *008887* Test Record Number: *3151*
Test Date: *03/30/2020* Test Time: *11:34am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:35am
FLO	Pass	11:35am
FC	Pass	11:35am

Temperature Tests

Test	Status	Time
FC1	Pass	11:35am
SRC	Pass	11:35am
DET	Pass	11:35am
BAR	Pass	11:35am
BT	Pass	11:35am

Blank Tests

Test	Status	Time
AIR	Pass	11:35am

Printer Tests

Test	Status	Time
PRNT	Pass	11:35am

CRC Tests

Test	Status	Time
COMP	Pass	11:36am
CAL	Pass	11:36am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Cleveland Instrument Location Kings Mountain PD

Instrument Serial No. 008900

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

CLEVELAND COUNTY KINGS MOUNTAIN PD 220

Serial Number: *008900*
Test Date: *03/30/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENENCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Hays, Mark D*
Permit Number: *0011-3099*
Effective:
11/13/2019-11/13/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG821801
Exp Date: 08/06/2020

Test	g/210L	Time
DIAG	Pass	12:45pm
AIR BLK	.00	12:46pm
ACCY CHK	.08	12:47pm
AIR BLK	.00	12:48pm
SUB TEST	**.00**	**12:49pm**
AIR BLK	.00	12:50pm
SUB TEST	**.00**	**12:52pm**
AIR BLK	.00	12:52pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CLEVELAND COUNTY KINGS MOUNTAIN PD 220

Serial Number: *008900* Test Record Number: *798*
Test Date: *03/30/2020* Test Time: *12:54pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:54pm
FLO	Pass	12:54pm
FC	Pass	12:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:55pm
SRC	Pass	12:55pm
DET	Pass	12:55pm
BAR	Pass	12:55pm
BT	Pass	12:55pm

Blank Tests

Test	Status	Time
AIR	Pass	12:55pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:55pm

CRC Tests

Test	Status	Time
COMP	Pass	12:55pm
CAL	Pass	12:55pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County CRAVEN Instrument Location CRAVEN COUNTY

Instrument Serial No. 008732 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 **day of** MARCH **, 20** 20**, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

CRAVEN COUNTY DETENTION CENTER 240

Serial Number: *008732*
Test Date: *03/24/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, ALVIN R*
Permit Number: *15671E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919901
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	10:52am
AIR BLK	.00	10:52am
ACCY CHK	.08	10:53am
AIR BLK	.00	10:54am
SUB TEST	**.00**	**10:54am**
AIR BLK	.00	10:55am
SUB TEST	**.00**	**10:57am**
AIR BLK	.00	10:57am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Alvin Ray Barnes

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY DETENTION CENTER 240

Serial Number: *008732* Test Record Number: *2384*
Test Date: *03/24/2020* Test Time: *11:00am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:00am
FLO	Pass	11:00am
FC	Pass	11:01am

Temperature Tests

Test	Status	Time
FC1	Pass	11:01am
SRC	Pass	11:01am
DET	Pass	11:01am
BAR	Pass	11:01am
BT	Pass	11:01am

Blank Tests

Test	Status	Time
AIR	Pass	11:01am

Printer Tests

Test	Status	Time
PRNT	Pass	11:01am

CRC Tests

Test	Status	Time
COMP	Pass	11:02am
CAL	Pass	11:02am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County CRAVEN Instrument Location HAVELOCK

Instrument Serial No. 008800 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of MARCH, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official — Certificate Number 648

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

CRAVEN COUNTY HAVELOCK PD 240

Serial Number: *008800*
Test Date: *03/24/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, ALVIN R*
Permit Number: *15671E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911501
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	3:19pm
AIR BLK	.00	3:20pm
ACCY CHK	.08	3:20pm
AIR BLK	.00	3:21pm
SUB TEST	**.00**	**3:22pm**
AIR BLK	.00	3:23pm
SUB TEST	**.00**	**3:24pm**
AIR BLK	.00	3:25pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Alvin R Barnes
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY HAVELOCK PD 240

Serial Number: *008800* Test Record Number: *1268*
Test Date: *03/24/2020* Test Time: *3:27pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:27pm
FLO	Pass	3:27pm
FC	Pass	3:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:27pm
SRC	Pass	3:27pm
DET	Pass	3:27pm
BAR	Pass	3:27pm
BT	Pass	3:27pm

Blank Tests

Test	Status	Time
AIR	Pass	3:28pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:28pm

CRC Tests

Test	Status	Time
COMP	Pass	3:28pm
CAL	Pass	3:28pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County CRAVEN Instrument Location NEW BERN POLICE DEPT

Instrument Serial No. 008817

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 **day of** MARCH **, 20** 20**, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Alan Ray Barnes
Signature of Certifying Official

C048
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

CRAVEN COUNTY NEW BERN PD 240

Serial Number: *008817*
Test Date: *03/24/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, ALVIN R*
Permit Number: *15671E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG920301
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	12:38pm
AIR BLK	.00	12:38pm
ACCY CHK	.07	12:39pm
AIR BLK	.00	12:41pm
SUB TEST	**.00**	**12:41pm**
AIR BLK	.00	12:42pm
SUB TEST	**.00**	**12:44pm**
AIR BLK	.00	12:45pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY NEW BERN PD 240

Serial Number: *008817* Test Record Number: *1542*
Test Date: *03/24/2020* Test Time: *12:45pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:45pm
FLO	Pass	12:45pm
FC	Pass	12:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:45pm
SRC	Pass	12:45pm
DET	Pass	12:45pm
BAR	Pass	12:45pm
BT	Pass	12:45pm

Blank Tests

Test	Status	Time
AIR	Pass	12:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:46pm

CRC Tests

Test	Status	Time
COMP	Pass	12:46pm
CAL	Pass	12:46pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County CRAVEN Instrument Location MCAS

Instrument Serial No. 010819 CHERRY POINT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 **day of** MARCH, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

CRAVEN COUNTY MCAS CHERRY POINT 240

Serial Number: *010819*
Test Date: *03/24/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, ALVIN R*
Permit Number: *15671E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG831801
Exp Date: 11/14/2020

Test	g/210L	Time
DIAG	Pass	4:08pm
AIR BLK	.00	4:08pm
ACCY CHK	.08	4:09pm
AIR BLK	.00	4:10pm
SUB TEST	**.00**	**4:11pm**
AIR BLK	.00	4:11pm
SUB TEST	**.00**	**4:13pm**
AIR BLK	.00	4:14pm

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

Alvin R Barnes
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY MCAS CHERRY POINT 240

Serial Number: *010819* Test Record Number: *608*
Test Date: *03/24/2020* Test Time: *4:14pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:14pm
FLO	Pass	4:15pm
FC	Pass	4:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:15pm
SRC	Pass	4:15pm
DET	Pass	4:15pm
BAR	Pass	4:15pm
BT	Pass	4:15pm

Blank Tests

Test	Status	Time
AIR	Pass	4:15pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:15pm

CRC Tests

Test	Status	Time
COMP	Pass	4:16pm
CAL	Pass	4:16pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County CURRITUCK Instrument Location CURRITUCK CO. S.O.

Instrument Serial No. 008947 407-A MAPLE Rd., Maple, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th **day of** MARCH, 20 21, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CURRITUCK COUNTY CURRITUCK SO-MAPLE 260

Serial Number: *008947*
Test Date: *03/20/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Linda A*
Permit Number: *0045-5468*
Effective:
07/08/2019-07/08/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG933703
Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	1:01pm
AIR BLK	.00	1:02pm
ACCY CHK	.08	1:03pm
AIR BLK	.00	1:04pm
SUB TEST	**.00**	**1:04pm**
AIR BLK	.00	1:05pm
SUB TEST	**.00**	**1:07pm**
AIR BLK	.00	1:08pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used ~~when performing~~ Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CURRITUCK COUNTY CURRITUCK SO-MAPLE 260

Serial Number: *008947* Test Record Number: *2589*
Test Date: *03/20/2020* Test Time: *1:08pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:09pm
FLO	Pass	1:09pm
FC	Pass	1:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:09pm
SRC	Pass	1:09pm
DET	Pass	1:09pm
BAR	Pass	1:09pm
BT	Pass	1:09pm

Blank Tests

Test	Status	Time
AIR	Pass	1:09pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:10pm

CRC Tests

Test	Status	Time
COMP	Pass	1:10pm
CAL	Pass	1:10pm

Preventive Maintenance
Status: Pass

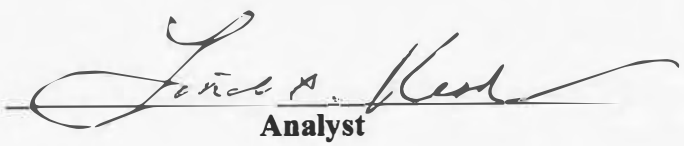

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Dare Instrument Location Dare Co. Detention Center

Instrument Serial No. 008783 1044 Driftwood Dr. Manteo NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd **day of** March **, 20**20**, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: *008783*
Test Date: *03/03/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *GUARD, KELLY G*
Permit Number: *12955E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919901
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	9:11am
AIR BLK	.00	9:12am
ACCY CHK	.07	9:13am
AIR BLK	.00	9:14am
SUB TEST	**.00**	**9:14am**
AIR BLK	.00	9:15am
SUB TEST	**.00**	**9:17am**
AIR BLK	.00	9:18am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: *008783* Test Record Number: *899*
Test Date: *03/03/2020* Test Time: *9:19am EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:19am
FLO	Pass	9:19am
FC	Pass	9:19am

Temperature Tests

Test	Status	Time
FC1	Pass	9:20am
SRC	Pass	9:20am
DET	Pass	9:20am
BAR	Pass	9:20am
BT	Pass	9:20am

Blank Tests

Test	Status	Time
AIR	Pass	9:20am

Printer Tests

Test	Status	Time
PRNT	Pass	9:20am

CRC Tests

Test	Status	Time
COMP	Pass	9:20am
CAL	Pass	9:20am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Dare Instrument Location Dare Co. Detention Center

Instrument Serial No. 008804 1644 Driftwood Dr. Manteo N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd **day of** March, **20** 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Ken — 643

Signature of Certifying Official — Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: *008804*
Test Date: *03/03/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *GUARD, KELLY G*
Permit Number: *12955E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG902106
Exp Date: 01/21/2021

Test	g/210L	Time
DIAG	Pass	8:56am
AIR BLK	.00	8:57am
ACCY CHK	.07	8:57am
AIR BLK	.00	8:58am
SUB TEST	**.00**	**8:59am**
AIR BLK	.00	9:00am
SUB TEST	**.00**	**9:01am**
AIR BLK	.00	9:02am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: *008804* Test Record Number: *2330*
Test Date: *03/03/2020* Test Time: *9:03am EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:04am
FLO	Pass	9:04am
FC	Pass	9:04am

Temperature Tests

Test	Status	Time
FC1	Pass	9:04am
SRC	Pass	9:04am
DET	Pass	9:04am
BAR	Pass	9:04am
BT	Pass	9:04am

Blank Tests

Test	Status	Time
AIR	Pass	9:05am

Printer Tests

Test	Status	Time
PRNT	Pass	9:05am

CRC Tests

Test	Status	Time
COMP	Pass	9:05am
CAL	Pass	9:05am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County DARE Instrument Location Kill Devil Hills P.D.

Instrument Serial No. 008844 102 Town Hall Dr., Kill Devil Hills, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th **day of** MARCH, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY KILL DEVIL HILLS PD 270

Serial Number: *008844*
Test Date: *03/05/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Linda A*
Permit Number: *0045-5468*
Effective:
07/08/2019-07/08/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG821801
Exp Date: 08/06/2020

Test	g/210L	Time
DIAG	Pass	9:02am
AIR BLK	.00	9:02am
ACCY CHK	.07	9:03am
AIR BLK	.00	9:04am
SUB TEST	**.00**	**9:05am**
AIR BLK	.00	9:06am
SUB TEST	**.00**	**9:07am**
AIR BLK	.00	9:08am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Linda A. Keesler
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY KILL DEVIL HILLS PD 270

Serial Number: *008844* Test Record Number: *2333*
Test Date: *03/05/2020* Test Time: *9:08am EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:09am
FLO	Pass	9:09am
FC	Pass	9:09am

Temperature Tests

Test	Status	Time
FC1	Pass	9:09am
SRC	Pass	9:09am
DET	Pass	9:09am
BAR	Pass	9:09am
BT	Pass	9:09am

Blank Tests

Test	Status	Time
AIR	Pass	9:10am

Printer Tests

Test	Status	Time
PRNT	Pass	9:10am

CRC Tests

Test	Status	Time
COMP	Pass	9:10am
CAL	Pass	9:10am

Preventive Maintenance
Status: Pass

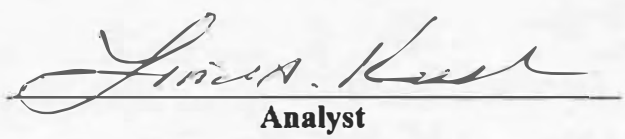

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County DUPLIN Instrument Location WALLACE POLICE DEPT

Instrument Serial No. 008858

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of MARCH, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

DUPLIN COUNTY WALLACE PD 300

Serial Number: *008858*
Test Date: *03/27/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, ALVIN R*
Permit Number: *15671E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919901
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	1:31pm
AIR BLK	.00	1:31pm
ACCY CHK	.08	1:32pm
AIR BLK	.00	1:33pm
SUB TEST	**.00**	**1:33pm**
AIR BLK	.00	1:34pm
SUB TEST	**.00**	**1:36pm**
AIR BLK	.00	1:36pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DUPLIN COUNTY WALLACE PD 300

Serial Number: *008858* Test Record Number: *1028*
Test Date: *03/27/2020* Test Time: *1:38pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:38pm
FLO	Pass	1:38pm
FC	Pass	1:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:38pm
SRC	Pass	1:38pm
DET	Pass	1:38pm
BAR	Pass	1:38pm
BT	Pass	1:38pm

Blank Tests

Test	Status	Time
AIR	Pass	1:39pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:39pm

CRC Tests

Test	Status	Time
COMP	Pass	1:39pm
CAL	Pass	1:39pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County DUPLIN Instrument Location DUPLIN COUNTY

Instrument Serial No. 008864 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of MARCH, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

DUPLIN COUNTY DETENTION CENTER 300

Serial Number: *008864*
Test Date: *03/27/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, ALVIN R*
Permit Number: *15671E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG934001
Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	2:59pm
AIR BLK	.00	3:00pm
ACCY CHK	.08	3:01pm
AIR BLK	.00	3:02pm
SUB TEST	**.00**	**3:03pm**
AIR BLK	.00	3:03pm
SUB TEST	**.00**	**3:05pm**
AIR BLK	.00	3:06pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DUPLIN COUNTY DETENTION CENTER 300

Serial Number: *008864* Test Record Number: *3841*
Test Date: *03/27/2020* Test Time: *3:07pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:07pm
FLO	Pass	3:07pm
FC	Pass	3:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:07pm
SRC	Pass	3:07pm
DET	Pass	3:07pm
BAR	Pass	3:07pm
BT	Pass	3:07pm

Blank Tests

Test	Status	Time
AIR	Pass	3:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:08pm

CRC Tests

Test	Status	Time
COMP	Pass	3:08pm
CAL	Pass	3:08pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County FRANKLIN Instrument Location FRANKLIN CO. LEC

Instrument Serial No. 008932 285 T KEMP RD LOUISBURG, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of MARCH, 20 20 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

B L D Smith 637

Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FRANKLIN COUNTY FRANKLIN CO. LEC 340

Serial Number: *008933*
Test Date: *03/10/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Smith, Brian D*
Permit Number: *0032-6608*
Effective:
07/09/2019-07/09/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919902
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	9:29am
AIR BLK	.00	9:29am
ACCY CHK	.07	9:30am
AIR BLK	.00	9:31am
SUB TEST	**.00**	**9:32am**
AIR BLK	.00	9:32am
SUB TEST	**.00**	**9:34am**
AIR BLK	.00	9:35am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FRANKLIN COUNTY FRANKLIN CO. LEC 340

Serial Number: *008933* Test Record Number: *1191*
Test Date: *03/10/2020* Test Time: *9:36am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:36am
FLO	Pass	9:36am
FC	Pass	9:36am

Temperature Tests

Test	Status	Time
FC1	Pass	9:36am
SRC	Pass	9:36am
DET	Pass	9:36am
BAR	Pass	9:36am
BT	Pass	9:36am

Blank Tests

Test	Status	Time
AIR	Pass	9:37am

Printer Tests

Test	Status	Time
PRNT	Pass	9:37am

CRC Tests

Test	Status	Time
COMP	Pass	9:37am
CAL	Pass	9:37am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County FRANKLIN Instrument Location FRANKLIN CO. LEC

Instrument Serial No. 008942 285 T KEMP RD LOUISBURG, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of MARCH, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

B. D. Smith
Signature of Certifying Official

637
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

FRANKLIN COUNTY FRANKLIN CO. LEC 340

Serial Number: *008942*
Test Date: *03/10/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Smith, Brian D*
Permit Number: *0032-6608*
Effective:
07/09/2019-07/09/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG934001
Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	9:09pm
AIR BLK	.00	9:09pm
ACCY CHK	.07	9:10pm
AIR BLK	.00	9:11pm
SUB TEST	**.00**	**9:11pm**
AIR BLK	.00	9:12pm
SUB TEST	**.00**	**9:14pm**
AIR BLK	.00	9:15pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FRANKLIN COUNTY FRANKLIN CO. LEC 340

Serial Number: *008942* Test Record Number: *1921*
Test Date: *03/10/2020* Test Time: *9:15pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:15pm
FLO	Pass	9:15pm
FC	Pass	9:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:16pm
SRC	Pass	9:16pm
DET	Pass	9:16pm
BAR	Pass	9:16pm
BT	Pass	9:16pm

Blank Tests

Test	Status	Time
AIR	Pass	9:16pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:16pm

CRC Tests

Test	Status	Time
COMP	Pass	9:16pm
CAL	Pass	9:16pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Gaston Instrument Location Gaston County

Instrument Serial No. 008643 Sheriffs Office

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of March, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: *008643*
Test Date: *03/23/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Hays, Mark D*
Permit Number: *0011-3099*
Effective:
11/13/2019-11/13/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG934001
Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	9:40am
AIR BLK	.00	9:41am
ACCY CHK	.07	9:42am
AIR BLK	.00	9:43am
SUB TEST	**.00**	**9:44am**
AIR BLK	.00	9:44am
SUB TEST	**.00**	**9:46am**
AIR BLK	.00	9:47am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: *008643* Test Record Number: *3478*
Test Date: *03/23/2020* Test Time: *9:49am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:49am
FLO	Pass	9:49am
FC	Pass	9:49am

Temperature Tests

Test	Status	Time
FC1	Pass	9:49am
SRC	Pass	9:49am
DET	Pass	9:49am
BAR	Pass	9:49am
BT	Pass	9:49am

Blank Tests

Test	Status	Time
AIR	Pass	9:50am

Printer Tests

Test	Status	Time
PRNT	Pass	9:50am

CRC Tests

Test	Status	Time
COMP	Pass	9:50am
CAL	Pass	9:50am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Gaston Instrument Location BAT Mobile Unit 2

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

658
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

GASTON COUNTY BAT MOBILE UNIT 02 350

Serial Number: *008970*
Test Date: *03/07/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *TOWERY, CHAD V*
Permit Number: *26632E*
Effective:
05/01/2019-05/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG807101
Exp Date: 03/12/2020

Test	g/210L	Time
DIAG	Pass	9:21pm
AIR BLK	.00	9:22pm
ACCY CHK	.08	9:22pm
AIR BLK	.00	9:23pm
SUB TEST	**.00**	**9:24pm**
AIR BLK	.00	9:25pm
SUB TEST	**.00**	**9:26pm**
AIR BLK	.00	9:27pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY BAT MOBILE UNIT 02 350

Serial Number: *008970* Test Record Number: *714*
Test Date: *03/07/2020* Test Time: *9:28pm EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:28pm
FLO	Pass	9:28pm
FC	Pass	9:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:29pm
SRC	Pass	9:29pm
DET	Pass	9:29pm
BAR	Pass	9:29pm
BT	Pass	9:29pm

Blank Tests

Test	Status	Time
AIR	Pass	9:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:29pm

CRC Tests

Test	Status	Time
COMP	Pass	9:29pm
CAL	Pass	9:29pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Gaston Instrument Location BAT Mobile Unit 2

Instrument Serial No. 009973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of March, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

658
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

GASTON COUNTY BAT MOBILE UNIT 02 350

Serial Number: *008973*
Test Date: *03/07/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *TOWERY, CHAD V*
Permit Number: *26632E*
Effective:
05/01/2019-05/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG807101
Exp Date: 03/12/2020

Test	g/210L	Time
DIAG	Pass	9:18pm
AIR BLK	.00	9:19pm
ACCY CHK	.08	9:20pm
AIR BLK	.00	9:21pm
SUB TEST	**.00**	**9:21pm**
AIR BLK	.00	9:22pm
SUB TEST	**.00**	**9:24pm**
AIR BLK	.00	9:25pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY BAT MOBILE UNIT 02 350

Serial Number: *008973* Test Record Number: *787*
Test Date: *03/07/2020* Test Time: *9:26pm EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:26pm
FLO	Pass	9:26pm
FC	Pass	9:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:26pm
SRC	Pass	9:26pm
DET	Pass	9:26pm
BAR	Pass	9:26pm
BT	Pass	9:26pm

Blank Tests

Test	Status	Time
AIR	Pass	9:27pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:27pm

CRC Tests

Test	Status	Time
COMP	Pass	9:27pm
CAL	Pass	9:27pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Gates Instrument Location Gates Co. S.O.

Instrument Serial No. 008884 202 Court St, Gatesville, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of March, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GATES COUNTY GATES CO SO 360

Serial Number: *008884*
Test Date: *03/18/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *GUARD, KELLY G*
Permit Number: *12955E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG814901
Exp Date: 05/29/2020

Test	g/210L	Time
DIAG	Pass	10:57am
AIR BLK	.00	10:57am
ACCY CHK	.07	10:58am
AIR BLK	.00	10:59am
SUB TEST	**.00**	**11:00am**
AIR BLK	.00	11:01am
SUB TEST	**.00**	**11:02am**
AIR BLK	.00	11:03am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GATES COUNTY GATES CO SO 360

Serial Number: *008884* Test Record Number: *942*
Test Date: *03/18/2020* Test Time: *11:04am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:05am
FLO	Pass	11:05am
FC	Pass	11:05am

Temperature Tests

Test	Status	Time
FC1	Pass	11:05am
SRC	Pass	11:05am
DET	Pass	11:05am
BAR	Pass	11:05am
BT	Pass	11:05am

Blank Tests

Test	Status	Time
AIR	Pass	11:05am

Printer Tests

Test	Status	Time
PRNT	Pass	11:06am

CRC Tests

Test	Status	Time
COMP	Pass	11:06am
CAL	Pass	11:06am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Graham Instrument Location Graham Co. SD

Instrument Serial No. 008915 Robbinsville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of March, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA MAY 20, 1775 APRIL 12, 1776 ESSE QUAM VIDERI

Neil R. Cutler — Signature of Certifying Official

635 — Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GRAHAM COUNTY GRAHAM COUNTY SD 370

Serial Number: *008915*
Test Date: *03/12/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
07/12/2019-07/12/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG920301
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	9:52am
AIR BLK	.00	9:53am
ACCY CHK	.08	9:54am
AIR BLK	.00	9:55am
SUB TEST	**.00**	**9:56am**
AIR BLK	.00	9:57am
SUB TEST	**.00**	**9:58am**
AIR BLK	.00	10:00am

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

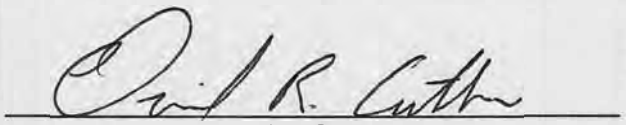

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GRAHAM COUNTY GRAHAM COUNTY SD 370

Serial Number: *008915* Test Record Number: *797*
Test Date: *03/12/2020* Test Time: *10:02am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:03am
FLO	Pass	10:03am
FC	Pass	10:03am

Temperature Tests

Test	Status	Time
FC1	Pass	10:03am
SRC	Pass	10:03am
DET	Pass	10:03am
BAR	Pass	10:03am
BT	Pass	10:03am

Blank Tests

Test	Status	Time
AIR	Pass	10:03am

Printer Tests

Test	Status	Time
PRNT	Pass	10:04am

CRC Tests

Test	Status	Time
COMP	Pass	10:04am
CAL	Pass	10:04am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Guilford Instrument Location Greensboro Jail

Instrument Serial No. 008638 Greensboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official — Certificate Number 649

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: *008638*
Test Date: *03/18/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BURNETTE, ANTHONY J*
Permit Number: *11304E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919902
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	2:00pm
AIR BLK	.00	2:00pm
ACCY CHK	.08	2:01pm
AIR BLK	.00	2:02pm
SUB TEST	**.00**	**2:03pm**
AIR BLK	.00	2:04pm
SUB TEST	**.00**	**2:05pm**
AIR BLK	.00	2:06pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court GVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: *008638* Test Record Number: *4463*
Test Date: *03/18/2020* Test Time: *2:08pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:09pm
FLO	Pass	2:09pm
FC	Pass	2:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:09pm
SRC	Pass	2:09pm
DET	Pass	2:09pm
BAR	Pass	2:09pm
BT	Pass	2:09pm

Blank Tests

Test	Status	Time
AIR	Pass	2:10pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:10pm

CRC Tests

Test	Status	Time
COMP	Pass	2:10pm
CAL	Pass	2:10pm

Preventive Maintenance
Status: Pass

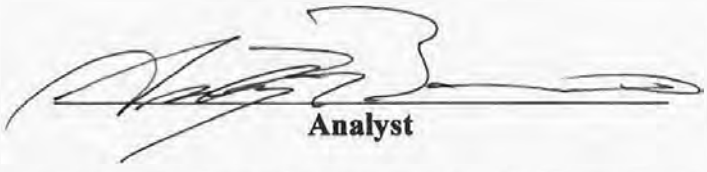

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Guilford Instrument Location Greensboro Jail

Instrument Serial No. 008790 Greensboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of March, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: *008790*
Test Date: *03/18/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BURNETTE, ANTHONY J*
Permit Number: *11304E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG920301
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	1:59pm
AIR BLK	.00	2:00pm
ACCY CHK	.08	2:00pm
AIR BLK	.00	2:02pm
SUB TEST	**.00**	**2:02pm**
AIR BLK	.00	2:03pm
SUB TEST	**.00**	**2:05pm**
AIR BLK	.00	2:06pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

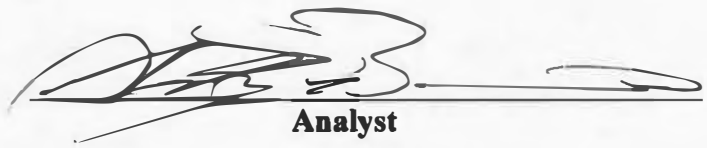

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: *008790* Test Record Number: *6806*
Test Date: *03/18/2020* Test Time: *2:10pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:10pm
FLO	Pass	2:10pm
FC	Pass	2:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:10pm
SRC	Pass	2:10pm
DET	Pass	2:10pm
BAR	Pass	2:10pm
BT	Pass	2:10pm

Blank Tests

Test	Status	Time
AIR	Pass	2:11pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:11pm

CRC Tests

Test	Status	Time
COMP	Pass	2:11pm
CAL	Pass	2:11pm

Preventive Maintenance
Status: Pass

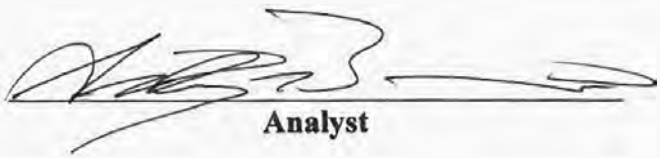

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Guilford Instrument Location Greensboro Jail

Instrument Serial No. 008754 Greensboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: *008794*
Test Date: *03/18/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BURNETTE, ANTHONY J*
Permit Number: *11304E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG920301
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	1:59pm
AIR BLK	.00	2:00pm
ACCY CHK	.08	2:01pm
AIR BLK	.00	2:02pm
SUB TEST	**.00**	**2:03pm**
AIR BLK	.00	2:03pm
SUB TEST	**.00**	**2:05pm**
AIR BLK	.00	2:06pm

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

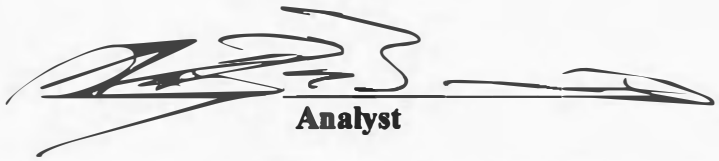

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: *008794* Test Record Number: *6837*
Test Date: *03/18/2020* Test Time: *2:09pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:10pm
FLO	Pass	2:10pm
FC	Pass	2:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:10pm
SRC	Pass	2:10pm
DET	Pass	2:10pm
BAR	Pass	2:10pm
BT	Pass	2:10pm

Blank Tests

Test	Status	Time
AIR	Pass	2:10pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:10pm

CRC Tests

Test	Status	Time
COMP	Pass	2:11pm
CAL	Pass	2:11pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Harnett Co. Instrument Location Dunn Police Dept

Instrument Serial No. 605644 Dunn, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

HARNETT COUNTY DUNN PD 420

Serial Number: *008644*
Test Date: *03/19/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911501
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	11:09am
AIR BLK	.00	11:10am
ACCY CHK	.07	11:11am
AIR BLK	.00	11:12am
SUB TEST	**.00**	**11:13am**
AIR BLK	.00	11:13am
SUB TEST	**.00**	**11:15am**
AIR BLK	.00	11:16am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HARNETT COUNTY DUNN PD 420

Serial Number: *008644* Test Record Number: *1425*
Test Date: *03/19/2020* Test Time: *11:16am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:17am
FLO	Pass	11:17am
FC	Pass	11:17am

Temperature Tests

Test	Status	Time
FC1	Pass	11:17am
SRC	Pass	11:17am
DET	Pass	11:17am
BAR	Pass	11:17am
BT	Pass	11:17am

Blank Tests

Test	Status	Time
AIR	Pass	11:17am

Printer Tests

Test	Status	Time
PRNT	Pass	11:17am

CRC Tests

Test	Status	Time
COMP	Pass	11:18am
CAL	Pass	11:18am

Preventive Maintenance
Status: Pass

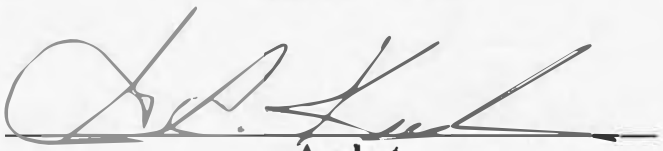

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County HARNETT Co. Instrument Location HARNETT Co. Detention Center

Instrument Serial No. 008129 Lillington, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of March, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human ~~Services, and~~ the instrument is functioning properly.

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HARNETT COUNTY DETENTION CENTER 420

Serial Number: *008729*
Test Date: *03/19/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911501
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	12:13pm
AIR BLK	.00	12:13pm
ACCY CHK	.08	12:14pm
AIR BLK	.00	12:15pm
SUB TEST	**.00**	**12:15pm**
AIR BLK	.00	12:16pm
SUB TEST	**.00**	**12:18pm**
AIR BLK	.00	12:19pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HARNETT COUNTY DETENTION CENTER 420

Serial Number: *008729* Test Record Number: *2372*
Test Date: *03/19/2020* Test Time: *12:19pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:19pm
FLO	Pass	12:19pm
FC	Pass	12:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:20pm
SRC	Pass	12:20pm
DET	Pass	12:20pm
BAR	Pass	12:20pm
BT	Pass	12:20pm

Blank Tests

Test	Status	Time
AIR	Pass	12:20pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:20pm

CRC Tests

Test	Status	Time
COMP	Pass	12:20pm
CAL	Pass	12:20pm

Preventive Maintenance
Status: Pass

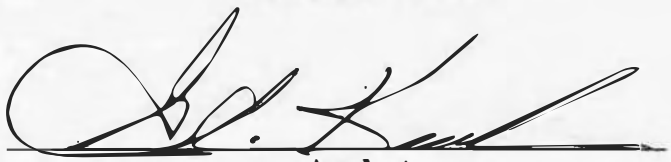

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Harnett Co. Instrument Location Harnett Co. Detention Center

Instrument Serial No. 008730 Lillington, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of March, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

HARNETT COUNTY DETENTION CENTER 420

Serial Number: *008730*
Test Date: *03/19/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAITENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911501
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	12:15pm
AIR BLK	.00	12:15pm
ACCY CHK	.08	12:16pm
AIR BLK	.00	12:17pm
SUB TEST	**.00**	**12:18pm**
AIR BLK	.00	12:19pm
SUB TEST	**.00**	**12:21pm**
AIR BLK	.00	12:21pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HARNETT COUNTY DETENTION CENTER 420

Serial Number: *008730* Test Record Number: *3417*
Test Date: *03/19/2020* Test Time: *12:22pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:22pm
FLO	Pass	12:22pm
FC	Pass	12:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:22pm
SRC	Pass	12:22pm
DET	Pass	12:22pm
BAR	Pass	12:22pm
BT	Pass	12:22pm

Blank Tests

Test	Status	Time
AIR	Pass	12:23pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:23pm

CRC Tests

Test	Status	Time
COMP	Pass	12:23pm
CAL	Pass	12:23pm

Preventive Maintenance
Status: Pass

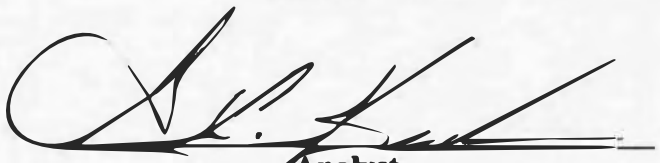

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Haywood Instrument Location Haywood Co. Jail

Instrument Serial No. 008712 Waynesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

David R. Cutler — Signature of Certifying Official

635 — Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HAYWOOD COUNTY HAYWOOD COUNTY JAIL 430

Serial Number: *008712*
Test Date: *03/27/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
07/12/2019-07/12/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG920301
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	10:54am
AIR BLK	.00	10:55am
ACCY CHK	.08	10:56am
AIR BLK	.00	10:57am
SUB TEST	**.00**	**10:57am**
AIR BLK	.00	10:58am
SUB TEST	**.00**	**11:00am**
AIR BLK	.00	11:01am

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

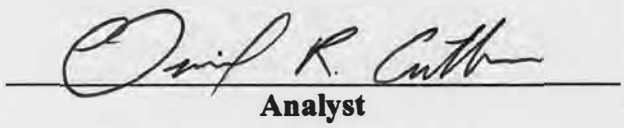

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HAYWOOD COUNTY HAYWOOD COUNTY JAIL 430

Serial Number: *008712* Test Record Number: *2276*
Test Date: *03/27/2020* Test Time: *11:02am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:03am
FLO	Pass	11:03am
FC	Pass	11:03am

Temperature Tests

Test	Status	Time
FC1	Pass	11:03am
SRC	Pass	11:03am
DET	Pass	11:03am
BAR	Pass	11:03am
BT	Pass	11:03am

Blank Tests

Test	Status	Time
AIR	Pass	11:03am

Printer Tests

Test	Status	Time
PRNT	Pass	11:04am

CRC Tests

Test	Status	Time
COMP	Pass	11:04am
CAL	Pass	11:04am

Preventive Maintenance
Status: Pass

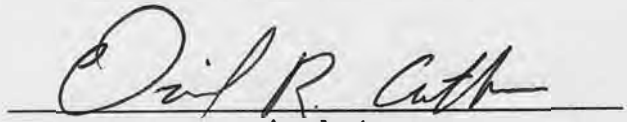

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Haywood Instrument Location Haywood Co. Jail

Instrument Serial No. 008714 Waynesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

David R. Luther — Signature of Certifying Official

635 — Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HAYWOOD COUNTY HAYWOOD COUNTY JAIL 430

Serial Number: *008714*
Test Date: *03/27/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
07/12/2019-07/12/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG821401
Exp Date: 08/02/2020

Test	g/210L	Time
DIAG	Pass	10:51am
AIR BLK	.00	10:52am
ACCY CHK	.07	10:53am
AIR BLK	.00	10:54am
SUB TEST	**.00**	**10:55am**
AIR BLK	.00	10:56am
SUB TEST	**.00**	**10:57am**
AIR BLK	.00	10:58am

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HAYWOOD COUNTY HAYWOOD COUNTY JAIL 430

Serial Number: *008714* Test Record Number: *1641*
Test Date: *03/27/2020* Test Time: *11:00am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:00am
FLO	Pass	11:00am
FC	Pass	11:00am

Temperature Tests

Test	Status	Time
FC1	Pass	11:00am
SRC	Pass	11:00am
DET	Pass	11:00am
BAR	Pass	11:00am
BT	Pass	11:00am

Blank Tests

Test	Status	Time
AIR	Pass	11:01am

Printer Tests

Test	Status	Time
PRNT	Pass	11:01am

CRC Tests

Test	Status	Time
COMP	Pass	11:01am
CAL	Pass	11:01am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Hertford Instrument Location Murfreesboro P.D.

Instrument Serial No. 008906 115 E. Broad St., Murfreesboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th **day of** March **, 20** 20**, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

HERTFORD COUNTY MURFREESBORO PD 450

Serial Number: *008906*
Test Date: *03/18/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *GUARD, KELLY G*
Permit Number: *12955E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG821401
Exp Date: 08/02/2020

Test	g/210L	Time
DIAG	Pass	12:26pm
AIR BLK	.00	12:27pm
ACCY CHK	.08	12:27pm
AIR BLK	.00	12:29pm
SUB TEST	**.00**	**12:29pm**
AIR BLK	.00	12:30pm
SUB TEST	**.00**	**12:32pm**
AIR BLK	.00	12:33pm

Reported AC: .00 g/210L

Signature of ~~Chemical Analyst~~

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HERTFORD COUNTY MURFREESBORO PD 450

Serial Number: *008906* Test Record Number: *756*
Test Date: *03/18/2020* Test Time: *12:34pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:34pm
FLO	Pass	12:34pm
FC	Pass	12:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:35pm
SRC	Pass	12:35pm
DET	Pass	12:35pm
BAR	Pass	12:35pm
BT	Pass	12:35pm

Blank Tests

Test	Status	Time
AIR	Pass	12:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:35pm

CRC Tests

Test	Status	Time
COMP	Pass	12:35pm
CAL	Pass	12:35pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Hoke Co. Instrument Location Hoke Co. Detention Center

Instrument Serial No. 008852 Raeford, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th **day of** March, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

HOKE COUNTY DETENTION CENTER 460

Serial Number: *008852*
Test Date: *03/18/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG920301
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	2:45pm
AIR BLK	.00	2:45pm
ACCY CHK	.08	2:46pm
AIR BLK	.00	2:47pm
SUB TEST	**.00**	**2:48pm**
AIR BLK	.00	2:48pm
SUB TEST	**.00**	**2:50pm**
AIR BLK	.00	2:51pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HOKE COUNTY DETENTION CENTER 460

Serial Number: *008852* Test Record Number: *1001*
Test Date: *03/18/2020* Test Time: *2:52pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:52pm
FLO	Pass	2:52pm
FC	Pass	2:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:52pm
SRC	Pass	2:52pm
DET	Pass	2:52pm
BAR	Pass	2:52pm
BT	Pass	2:52pm

Blank Tests

Test	Status	Time
AIR	Pass	2:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:53pm

CRC Tests

Test	Status	Time
COMP	Pass	2:53pm
CAL	Pass	2:53pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Hoke Co. Instrument Location Hoke Co Detention Center

Instrument Serial No. 008853 Raeford, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th **day of** March, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HOKE COUNTY DETENTION CENTER 460

Serial Number: *008855*
Test Date: *03/18/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG920301
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	2:46pm
AIR BLK	.00	2:47pm
ACCY CHK	.08	2:47pm
AIR BLK	.00	2:49pm
SUB TEST	**.00**	**2:49pm**
AIR BLK	.00	2:50pm
SUB TEST	**.00**	**2:52pm**
AIR BLK	.00	2:53pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HOKE COUNTY DETENTION CENTER 460

Serial Number: *008855* Test Record Number: *1559*
Test Date: *03/18/2020* Test Time: *2:54pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:54pm
FLO	Pass	2:54pm
FC	Pass	2:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:54pm
SRC	Pass	2:54pm
DET	Pass	2:54pm
BAR	Pass	2:54pm
BT	Pass	2:54pm

Blank Tests

Test	Status	Time
AIR	Pass	2:55pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:55pm

CRC Tests

Test	Status	Time
COMP	Pass	2:55pm
CAL	Pass	2:55pm

Preventive Maintenance Status: Pass

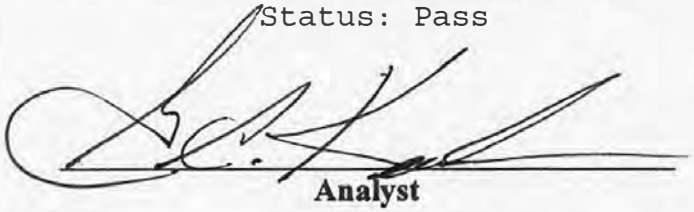

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Iredell Instrument Location Iredell County

Instrument Serial No. 008809 Sheriffs Office

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of March, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY IREDELL COUNTY SO 480

Serial Number: *008809*
Test Date: *03/19/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Hays, Mark D*
Permit Number: *0011-3099*
Effective:
11/13/2019-11/13/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919901
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	9:46am
AIR BLK	.00	9:47am
ACCY CHK	.08	9:48am
AIR BLK	.00	9:49am
SUB TEST	**.00**	**9:49am**
AIR BLK	.00	9:50am
SUB TEST	**.00**	**9:51am**
AIR BLK	.00	9:52am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY IREDELL COUNTY SO 480

Serial Number: *008809* Test Record Number: *4378*
Test Date: *03/19/2020* Test Time: *9:54am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:54am
FLO	Pass	9:54am
FC	Pass	9:54am

Temperature Tests

Test	Status	Time
FC1	Pass	9:55am
SRC	Pass	9:55am
DET	Pass	9:55am
BAR	Pass	9:55am
BT	Pass	9:55am

Blank Tests

Test	Status	Time
AIR	Pass	9:55am

Printer Tests

Test	Status	Time
PRNT	Pass	9:55am

CRC Tests

Test	Status	Time
COMP	Pass	9:55am
CAL	Pass	9:55am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Iredell Instrument Location Statesville PD

Instrument Serial No. 008910 300 S. Tradd St., Statesville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of March, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY STATESVILLE PD 480

Serial Number: *008910*
Test Date: *03/03/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Hays, Mark D*
Permit Number: *0011-3099*
Effective:
11/13/2019-11/13/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG814901
Exp Date: 05/29/2020

Test	g/210L	Time
DIAG	Pass	11:30am
AIR BLK	.00	11:31am
ACCY CHK	.07	11:32am
AIR BLK	.00	11:33am
SUB TEST	**.00**	**11:33am**
AIR BLK	.00	11:34am
SUB TEST	**.00**	**11:36am**
AIR BLK	.00	11:37am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY STATESVILLE PD 480

Serial Number: *008910* Test Record Number: *1064*
Test Date: *03/03/2020* Test Time: *11:38am EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:38am
FLO	Pass	11:38am
FC	Pass	11:38am

Temperature Tests

Test	Status	Time
FC1	Pass	11:38am
SRC	Pass	11:38am
DET	Pass	11:38am
BAR	Pass	11:38am
BT	Pass	11:38am

Blank Tests

Test	Status	Time
AIR	Pass	11:39am

Printer Tests

Test	Status	Time
PRNT	Pass	11:39am

CRC Tests

Test	Status	Time
COMP	Pass	11:39am
CAL	Pass	11:39am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Jackson Instrument Location Jackson Co. Jail

Instrument Serial No. 008708 Sylva, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

JACKSON COUNTY JACKSON COUNTY JAIL 490

Serial Number: *008708*
Test Date: *03/06/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
07/12/2019-07/12/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911506
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	11:05am
AIR BLK	.00	11:06am
ACCY CHK	.08	11:06am
AIR BLK	.00	11:07am
SUB TEST	**.00**	**11:08am**
AIR BLK	.00	11:09am
SUB TEST	**.00**	**11:10am**
AIR BLK	.00	11:11am

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JACKSON COUNTY JACKSON COUNTY JAIL 490

Serial Number: *008708* Test Record Number: *1490*
Test Date: *03/06/2020* Test Time: *11:12am EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:12am
FLO	Pass	11:12am
FC	Pass	11:12am

Temperature Tests

Test	Status	Time
FC1	Pass	11:13am
SRC	Pass	11:13am
DET	Pass	11:13am
BAR	Pass	11:13am
BT	Pass	11:13am

Blank Tests

Test	Status	Time
AIR	Pass	11:13am

Printer Tests

Test	Status	Time
PRNT	Pass	11:13am

CRC Tests

Test	Status	Time
COMP	Pass	11:13am
CAL	Pass	11:13am

Preventive Maintenance
Status: Pass

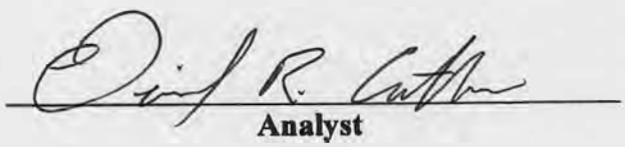

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Jackson Instrument Location Jackson Co. Jail

Instrument Serial No. 008722 Sylva, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th **day of** March, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA
MAY 20, 1775
APRIL 12, 1776
ESSE QUAM VIDERI

David R. Cutler — 635

Signature of Certifying Official — Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JACKSON COUNTY JACKSON COUNTY JAIL 490

Serial Number: *008722*
Test Date: *03/06/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
07/12/2019-07/12/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG920301
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	11:06am
AIR BLK	.00	11:07am
ACCY CHK	.08	11:07am
AIR BLK	.00	11:08am
SUB TEST	**.00**	**11:09am**
AIR BLK	.00	11:10am
SUB TEST	**.00**	**11:11am**
AIR BLK	.00	11:13am

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JACKSON COUNTY JACKSON COUNTY JAIL 490

Serial Number: *008722* Test Record Number: *1199*
Test Date: *03/06/2020* Test Time: *11:14am EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:15am
FLO	Pass	11:15am
FC	Pass	11:15am

Temperature Tests

Test	Status	Time
FC1	Pass	11:15am
SRC	Pass	11:15am
DET	Pass	11:15am
BAR	Pass	11:15am
BT	Pass	11:15am

Blank Tests

Test	Status	Time
AIR	Pass	11:16am

Printer Tests

Test	Status	Time
PRNT	Pass	11:16am

CRC Tests

Test	Status	Time
COMP	Pass	11:16am
CAL	Pass	11:16am

Preventive Maintenance
Status: Pass

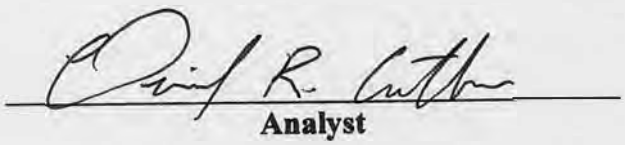

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Johnston Co. Instrument Location Selma Police Dept

Instrument Serial No. CO8595 Selma, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd **day of** March, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY SELMA PD 500

Serial Number: *008595*
Test Date: *03/02/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911501
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	9:58am
AIR BLK	.00	9:58am
ACCY CHK	.07	9:59am
AIR BLK	.00	10:00am
SUB TEST	**.00**	**10:01am**
AIR BLK	.00	10:02am
SUB TEST	**.00**	**10:03am**
AIR BLK	.00	10:04am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY SELMA PD 500

Serial Number: *008595* Test Record Number: *1423*
Test Date: *03/02/2020* Test Time: *10:05am EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:05am
FLO	Pass	10:05am
FC	Pass	10:05am

Temperature Tests

Test	Status	Time
FC1	Pass	10:05am
SRC	Pass	10:05am
DET	Pass	10:05am
BAR	Pass	10:05am
BT	Pass	10:05am

Blank Tests

Test	Status	Time
AIR	Pass	10:06am

Printer Tests

Test	Status	Time
PRNT	Pass	10:06am

CRC Tests

Test	Status	Time
COMP	Pass	10:06am
CAL	Pass	10:06am

Preventive Maintenance
Status: Pass

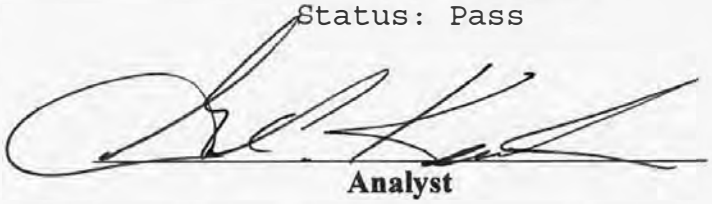

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Johnston Co. Instrument Location Benson Police Dept.

Instrument Serial No. 008885 Benson, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th **day of** March, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BENSON PD 500

Serial Number: *008885*
Test Date: *03/19/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911501
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	10:24am
AIR BLK	.00	10:24am
ACCY CHK	.08	10:25am
AIR BLK	.00	10:26am
SUB TEST	**.00**	**10:26am**
AIR BLK	.00	10:27am
SUB TEST	**.00**	**10:29am**
AIR BLK	.00	10:30am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BENSON PD 500

Serial Number: *008885* Test Record Number: *584*
Test Date: *03/19/2020* Test Time: *10:30am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:31am
FLO	Pass	10:31am
FC	Pass	10:31am

Temperature Tests

Test	Status	Time
FC1	Pass	10:31am
SRC	Pass	10:31am
DET	Pass	10:31am
BAR	Pass	10:31am
BT	Pass	10:31am

Blank Tests

Test	Status	Time
AIR	Pass	10:31am

Printer Tests

Test	Status	Time
PRNT	Pass	10:31am

CRC Tests

Test	Status	Time
COMP	Pass	10:32am
CAL	Pass	10:32am

Preventive Maintenance
Status: Pass

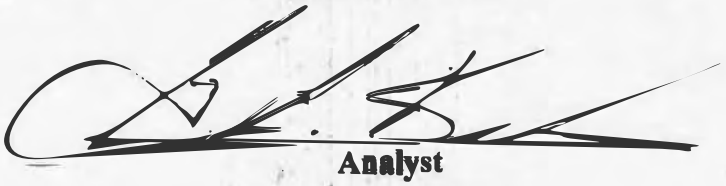

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County JONES Instrument Location JONES COUNTY

Instrument Serial No. 008705 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 **day of** MARCH **, 20** 20**, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official — Certificate Number 648

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

JONES COUNTY DETENTION CENTER 510

Serial Number: *008705*
Test Date: *03/27/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, ALVIN R*
Permit Number: *15671E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG934001
Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	11:02am
AIR BLK	.00	11:03am
ACCY CHK	.07	11:04am
AIR BLK	.00	11:05am
SUB TEST	**.00**	**11:06am**
AIR BLK	.00	11:07am
SUB TEST	**.00**	**11:08am**
AIR BLK	.00	11:09am

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

Alvin R Barnes
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JONES COUNTY DETENTION CENTER 510

Serial Number: *008705* Test Record Number: *1418*
Test Date: *03/27/2020* Test Time: *11:10am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:11am
FLO	Pass	11:11am
FC	Pass	11:11am

Temperature Tests

Test	Status	Time
FC1	Pass	11:11am
SRC	Pass	11:11am
DET	Pass	11:11am
BAR	Pass	11:11am
BT	Pass	11:11am

Blank Tests

Test	Status	Time
AIR	Pass	11:12am

Printer Tests

Test	Status	Time
PRNT	Pass	11:12am

CRC Tests

Test	Status	Time
COMP	Pass	11:12am
CAL	Pass	11:12am

Preventive Maintenance
Status: Pass

Allen Ray Barnes
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Lee Co. Instrument Location Lee Co Jail

Instrument Serial No. 008645 Sanford, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd **day of** March, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

LEE COUNTY DETENTION CENTER 520

Serial Number: *008645*
Test Date: *03/02/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911501
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	1:44pm
AIR BLK	.00	1:45pm
ACCY CHK	.08	1:45pm
AIR BLK	.00	1:46pm
SUB TEST	**.00**	**1:47pm**
AIR BLK	.00	1:48pm
SUB TEST	**.00**	**1:49pm**
AIR BLK	.00	1:50pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LEE COUNTY DETENTION CENTER 520

Serial Number: *008645* Test Record Number: *2001*
Test Date: *03/02/2020* Test Time: *1:51pm EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:51pm
FLO	Pass	1:51pm
FC	Pass	1:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:51pm
SRC	Pass	1:51pm
DET	Pass	1:51pm
BAR	Pass	1:51pm
BT	Pass	1:51pm

Blank Tests

Test	Status	Time
AIR	Pass	1:52pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:52pm

CRC Tests

Test	Status	Time
COMP	Pass	1:52pm
CAL	Pass	1:52pm

Preventive Maintenance
Status: Pass

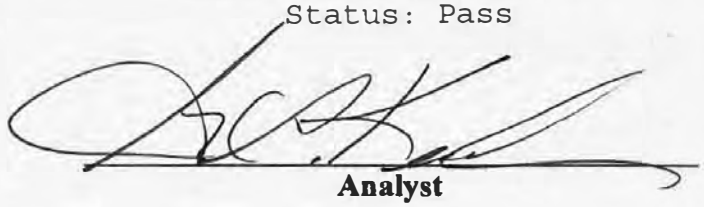

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Lee Co. Instrument Location Sanford Police Dept.

Instrument Serial No. 108867 Sanford NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd **day of** March **, 20**20**, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

LEE COUNTY SANFORD POLICE DEPT 520

Serial Number: *008867*
Test Date: *03/02/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG934001
Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	12:50pm
AIR BLK	.00	12:51pm
ACCY CHK	.08	12:52pm
AIR BLK	.00	12:53pm
SUB TEST	**.00**	**12:53pm**
AIR BLK	.00	12:54pm
SUB TEST	**.00**	**12:56pm**
AIR BLK	.00	12:57pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LEE COUNTY SANFORD POLICE DEPT 520

Serial Number: *008862* Test Record Number: *1150*
Test Date: *03/02/2020* Test Time: *12:57pm EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:58pm
FLC	Pass	12:58pm
FC	Pass	12:58pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:58pm
SRC	Pass	12:58pm
DET	Pass	12:58pm
BAR	Pass	12:58pm
BT	Pass	12:58pm

Blank Tests

Test	Status	Time
AIR	Pass	12:58pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:58pm

CRC Tests

Test	Status	Time
COMP	Pass	12:59pm
CAL	Pass	12:59pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County LENOIR Instrument Location KINSTON P.D.

Instrument Serial No. 008624 205 E. KNIGHT ST, KINSTON, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th **day of** MARCH, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LENOIR COUNTY KINSTON PD 530

Serial Number: *008624*
Test Date: *03/26/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Linda A*
Permit Number: *0045-5468*
Effective:
07/08/2019-07/08/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG933703
Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	1:38pm
AIR BLK	.00	1:39pm
ACCY CHK	.07	1:39pm
AIR BLK	.00	1:40pm
SUB TEST	**.00**	**1:41pm**
AIR BLK	.00	1:42pm
SUB TEST	**.00**	**1:43pm**
AIR BLK	.00	1:44pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY KINSTON PD 530

Serial Number: *008624* Test Record Number: *1833*
Test Date: *03/26/2020* Test Time: *1:44pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:45pm
FLO	Pass	1:45pm
FC	Pass	1:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:45pm
SRC	Pass	1:45pm
DET	Pass	1:45pm
BAR	Pass	1:45pm
BT	Pass	1:45pm

Blank Tests

Test	Status	Time
AIR	Pass	1:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:46pm

CRC Tests

Test	Status	Time
COMP	Pass	1:46pm
CAL	Pass	1:46pm

Preventive Maintenance
Status: Pass

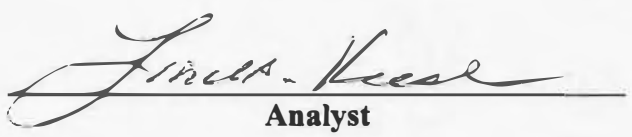

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Lincoln Instrument Location Lincoln County Courthouse

Instrument Serial No. 008823 #1 Court Square, Lincolnton

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Joseph E. Hutchins
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

LINCOLN COUNTY COURTHOUSE 540

Serial Number: *008823*
Test Date: *03/18/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Hutchinson, Joseph E*
Permit Number: *0035-6075*
Effective:
07/09/2019-07/09/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919901
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	1:15pm
AIR BLK	.00	1:15pm
ACCY CHK	.08	1:16pm
AIR BLK	.00	1:17pm
SUB TEST	**.00**	**1:18pm**
AIR BLK	.00	1:19pm
SUB TEST	**.00**	**1:20pm**
AIR BLK	.00	1:21pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LINCOLN COUNTY COURTHOUSE 540

Serial Number: *008823* Test Record Number: *1599*
Test Date: *03/18/2020* Test Time: *1:22pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:22pm
FLO	Pass	1:22pm
FC	Pass	1:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:22pm
SRC	Pass	1:22pm
DET	Pass	1:22pm
BAR	Pass	1:22pm
BT	Pass	1:22pm

Blank Tests

Test	Status	Time
AIR	Pass	1:23pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:23pm

CRC Tests

Test	Status	Time
COMP	Pass	1:23pm
CAL	Pass	1:23pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Lincoln Instrument Location Lincoln County Courthouse

Instrument Serial No. 008823 #1 Court Square, Lincolnton

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Joseph E. Hutchins
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

LINCOLN COUNTY COURTHOUSE 540

Serial Number: *008823*
Test Date: *03/18/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Hutchinson, Joseph E*
Permit Number: *0035-6075*
Effective:
07/09/2019-07/09/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919901
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	1:15pm
AIR BLK	.00	1:15pm
ACCY CHK	.08	1:16pm
AIR BLK	.00	1:17pm
SUB TEST	**.00**	**1:18pm**
AIR BLK	.00	1:19pm
SUB TEST	**.00**	**1:20pm**
AIR BLK	.00	1:21pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LINCOLN COUNTY COURTHOUSE 540

Serial Number: *008823* Test Record Number: *1599*
Test Date: *03/18/2020* Test Time: *1:22pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:22pm
FLO	Pass	1:22pm
FC	Pass	1:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:22pm
SRC	Pass	1:22pm
DET	Pass	1:22pm
BAR	Pass	1:22pm
BT	Pass	1:22pm

Blank Tests

Test	Status	Time
AIR	Pass	1:23pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:23pm

CRC Tests

Test	Status	Time
COMP	Pass	1:23pm
CAL	Pass	1:23pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Macon Instrument Location Macon Co. Jail

Instrument Serial No. 008618 Franklin, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

David R. Cattlin — Signature of Certifying Official

635 — Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MACON COUNTY MACON COUNTY JAIL 550

Serial Number: *008618*
Test Date: *03/24/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
07/12/2019-07/12/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919901
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	10:33am
AIR BLK	.00	10:34am
ACCY CHK	.08	10:35am
AIR BLK	.00	10:36am
SUB TEST	**.00**	**10:37am**
AIR BLK	.00	10:38am
SUB TEST	**.00**	**10:39am**
AIR BLK	.00	10:40am

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

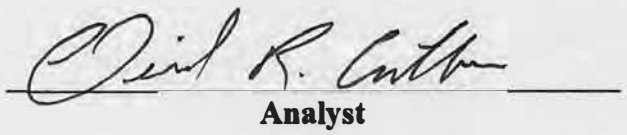

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MACON COUNTY MACON COUNTY JAIL 550

Serial Number: *008618* Test Record Number: *2027*
Test Date: *03/24/2020* Test Time: *10:42am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:42am
FLO	Pass	10:42am
FC	Pass	10:42am

Temperature Tests

Test	Status	Time
FC1	Pass	10:42am
SRC	Pass	10:42am
DET	Pass	10:42am
BAR	Pass	10:42am
BT	Pass	10:42am

Blank Tests

Test	Status	Time
AIR	Pass	10:43am

Printer Tests

Test	Status	Time
PRNT	Pass	10:43am

CRC Tests

Test	Status	Time
COMP	Pass	10:43am
CAL	Pass	10:43am

Preventive Maintenance
Status: Pass

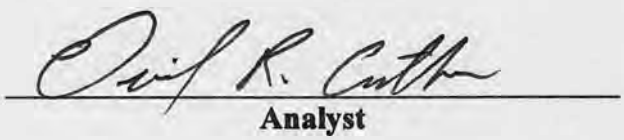

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Macon Instrument Location Macon Co. Jail

Instrument Serial No. 008789 Franklin, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Paul R. Cuthbertson — Signature of Certifying Official

635 — Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MACON COUNTY MACON COUNTY JAIL 550

Serial Number: *008789*
Test Date: *03/24/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
07/12/2019-07/12/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG902106
Exp Date: 01/21/2021

Test	g/210L	Time
DIAG	Pass	10:34am
AIR BLK	.00	10:35am
ACCY CHK	.07	10:36am
AIR BLK	.00	10:37am
SUB TEST	**.00**	**10:38am**
AIR BLK	.00	10:39am
SUB TEST	**.00**	**10:40am**
AIR BLK	.00	10:41am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MACON COUNTY MACON COUNTY JAIL 550

Serial Number: *008789* Test Record Number: *681*
Test Date: *03/24/2020* Test Time: *10:43am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:43am
FLO	Pass	10:43am
FC	Pass	10:43am

Temperature Tests

Test	Status	Time
FC1	Pass	10:43am
SRC	Pass	10:43am
DET	Pass	10:43am
BAR	Pass	10:43am
BT	Pass	10:43am

Blank Tests

Test	Status	Time
AIR	Pass	10:44am

Printer Tests

Test	Status	Time
PRNT	Pass	10:44am

CRC Tests

Test	Status	Time
COMP	Pass	10:44am
CAL	Pass	10:44am

Preventive Maintenance
Status: Pass

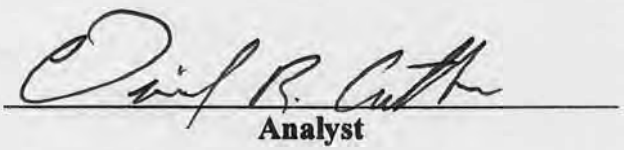

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Macon Instrument Location Macon Co. Magistrate

Instrument Serial No. 008795 Highlands, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

David R. Cuthrell — Signature of Certifying Official

635 — Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MACON COUNTY MACON CO MAGISTRATE 550

Serial Number: *008795*
Test Date: *03/23/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
07/12/2019-07/12/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG902106
Exp Date: 01/21/2021

Test	g/210L	Time
DIAG	Pass	2:12pm
AIR BLK	.00	2:13pm
ACCY CHK	.07	2:14pm
AIR BLK	.00	2:14pm
SUB TEST	**.00**	**2:15pm**
AIR BLK	.00	2:16pm
SUB TEST	**.00**	**2:18pm**
AIR BLK	.00	2:18pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Daniel R. Cutler
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MACON COUNTY MACON CO MAGISTRATE 550

Serial Number: *008795* Test Record Number: *488*
Test Date: *03/23/2020* Test Time: *2:20pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:20pm
FLO	Pass	2:20pm
FC	Pass	2:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:20pm
SRC	Pass	2:20pm
DET	Pass	2:20pm
BAR	Pass	2:20pm
BT	Pass	2:20pm

Blank Tests

Test	Status	Time
AIR	Pass	2:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:21pm

CRC Tests

Test	Status	Time
COMP	Pass	2:21pm
CAL	Pass	2:21pm

Preventive Maintenance
Status: Pass

David R. Cutlow

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Mecklenburg Instrument Location CMPD-LEC

Instrument Serial No. 008594 601 E. Trade St., Charlotte

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of March, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: *008594*
Test Date: *03/04/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Hays, Mark D*
Permit Number: *0011-3099*
Effective:
11/13/2019-11/13/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919902
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	11:05am
AIR BLK	.00	11:06am
ACCY CHK	.07	11:06am
AIR BLK	.00	11:07am
SUB TEST	**.00**	**11:08am**
AIR BLK	.00	11:09am
SUB TEST	**.00**	**11:11am**
AIR BLK	.00	11:11am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: *008594* Test Record Number: *4599*
Test Date: *03/04/2020* Test Time: *11:12am EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:13am
FLO	Pass	11:13am
FC	Pass	11:13am

Temperature Tests

Test	Status	Time
FC1	Pass	11:13am
SRC	Pass	11:13am
DET	Pass	11:13am
BAR	Pass	11:13am
BT	Pass	11:13am

Blank Tests

Test	Status	Time
AIR	Pass	11:14am

Printer Tests

Test	Status	Time
PRNT	Pass	11:14am

CRC Tests

Test	Status	Time
COMP	Pass	11:14am
CAL	Pass	11:14am

Preventive Maintenance
Status: Pass

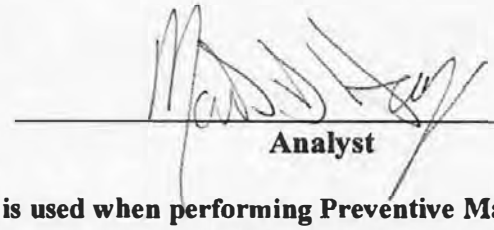

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Mecklenburg Instrument Location Mecklenburg Cant/ Sheriffs Office

Instrument Serial No. 008665

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of March, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY SHERIFFS OFFICE 590

Serial Number: *008665*
Test Date: *03/04/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Hays, Mark D*
Permit Number: *0011-3099*
Effective:
11/13/2019-11/13/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG933901
Exp Date: 12/05/2021

Test	g/210L	Time
DIAG	Pass	10:22am
AIR BLK	.00	10:23am
ACCY CHK	.08	10:24am
AIR BLK	.00	10:25am
SUB TEST	**.00**	**10:26am**
AIR BLK	.00	10:27am
SUB TEST	**.00**	**10:29am**
AIR BLK	.00	10:30am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY SHERIFFS OFFICE 590

Serial Number: *008665* Test Record Number: *4818*
Test Date: *03/04/2020* Test Time: *10:38am EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:39am
FLO	Pass	10:39am
FC	Pass	10:39am

Temperature Tests

Test	Status	Time
FC1	Pass	10:39am
SRC	Pass	10:39am
DET	Pass	10:39am
BAR	Pass	10:39am
BT	Pass	10:39am

Blank Tests

Test	Status	Time
AIR	Pass	10:40am

Printer Tests

Test	Status	Time
PRNT	Pass	10:40am

CRC Tests

Test	Status	Time
COMP	Pass	10:40am
CAL	Pass	10:40am

Preventive Maintenance
Status: Pass

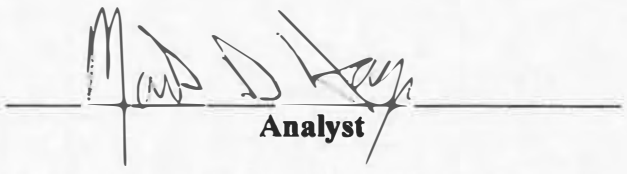

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Mecklenburg Instrument Location Huntersville Police Department

Instrument Serial No. 008747 9630 Julian Clark Ave.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of March, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG HUNTERSVILLE PD 590

Serial Number: *008747*
Test Date: *03/18/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Hays, Mark D*
Permit Number: *0011-3099*
Effective:
11/13/2019-11/13/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG821401
Exp Date: 08/02/2020

Test	g/210L	Time
DIAG	Pass	12:59pm
AIR BLK	.00	1:00pm
ACCY CHK	.08	1:01pm
AIR BLK	.00	1:02pm
SUB TEST	**.00**	**1:03pm**
AIR BLK	.00	1:04pm
SUB TEST	**.00**	**1:06pm**
AIR BLK	.00	1:06pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG HUNTERSVILLE PD 590

Serial Number: *008747* Test Record Number: *2767*
Test Date: *03/18/2020* Test Time: *1:08pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:08pm
FLO	Pass	1:08pm
FC	Pass	1:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:08pm
SRC	Pass	1:08pm
DET	Pass	1:08pm
BAR	Pass	1:08pm
BT	Pass	1:08pm

Blank Tests

Test	Status	Time
AIR	Pass	1:09pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:09pm

CRC Tests

Test	Status	Time
COMP	Pass	1:09pm
CAL	Pass	1:09pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Montgomery Co. Instrument Location Montgomery Co Detention Center

Instrument Serial No. 008657 Troy, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th **day of** March, 2022, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MONTGOMERY COUNTY DETENTION CENTER 610

Serial Number: *008657*
Test Date: *03/25/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911506
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	3:09pm
AIR BLK	.00	3:10pm
ACCY CHK	.08	3:10pm
AIR BLK	.00	3:11pm
SUB TEST	**.00**	**3:12pm**
AIR BLK	.00	3:13pm
SUB TEST	**.00**	**3:15pm**
AIR BLK	.00	3:15pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MONTGOMERY COUNTY DETENTION CENTER 610

Serial Number: *008657* Test Record Number: *1685*
Test Date: *03/25/2020* Test Time: *3:16pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:16pm
FLO	Pass	3:16pm
FC	Pass	3:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:16pm
SRC	Pass	3:16pm
DET	Pass	3:16pm
BAR	Pass	3:16pm
BT	Pass	3:16pm

Blank Tests

Test	Status	Time
AIR	Pass	3:17pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:17pm

CRC Tests

Test	Status	Time
COMP	Pass	3:17pm
CAL	Pass	3:17pm

Preventive Maintenance
Status: Pass

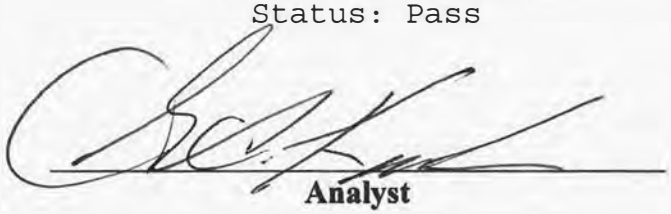

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Montgomery Co. Instrument Location Montgomery Co Detention Center

Instrument Serial No. 008092 Troy, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th day of March, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

MONTGOMERY COUNTY DETENTION CENTER 610

Serial Number: *008709*
Test Date: *03/25/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919902
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	3:07pm
AIR BLK	.00	3:08pm
ACCY CHK	.07	3:09pm
AIR BLK	.00	3:10pm
SUB TEST	**.00**	**3:11pm**
AIR BLK	.00	3:11pm
SUB TEST	**.00**	**3:13pm**
AIR BLK	.00	3:14pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MONTGOMERY COUNTY DETENTION CENTER 610

Serial Number: *008709* Test Record Number: *1212*
Test Date: *03/25/2020* Test Time: *3:14pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:15pm
FLO	Pass	3:15pm
FC	Pass	3:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:15pm
SRC	Pass	3:15pm
DET	Pass	3:15pm
BAR	Pass	3:15pm
BT	Pass	3:15pm

Blank Tests

Test	Status	Time
AIR	Pass	3:15pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:16pm

CRC Tests

Test	Status	Time
COMP	Pass	3:16pm
CAL	Pass	3:16pm

Preventive Maintenance
Status: Pass

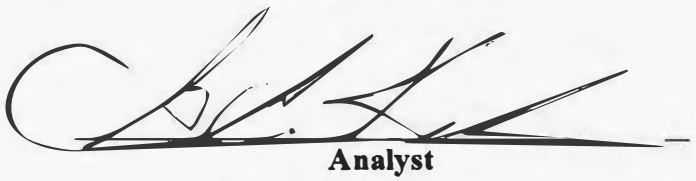

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Moore Co. Instrument Location Pinehurst Police Dept

Instrument Serial No. 005110 Pinehurst, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of March, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

MOORE COUNTY PINEHURST PD 620

Serial Number: *008710*
Test Date: *03/12/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911501
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	10:23am
AIR BLK	.00	10:24am
ACCY CHK	.07	10:24am
AIR BLK	.00	10:25am
SUB TEST	**.00**	**10:26am**
AIR BLK	.00	10:27am
SUB TEST	**.00**	**10:28am**
AIR BLK	.00	10:29am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MOORE COUNTY PINEHURST PD 620

Serial Number: *008710* Test Record Number: *1659*
Test Date: *03/12/2020* Test Time: *10:30am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:31am
FLO	Pass	10:31am
FC	Pass	10:31am

Temperature Tests

Test	Status	Time
FC1	Pass	10:31am
SRC	Pass	10:31am
DET	Pass	10:31am
BAR	Pass	10:31am
BT	Pass	10:31am

Blank Tests

Test	Status	Time
AIR	Pass	10:31am

Printer Tests

Test	Status	Time
PRNT	Pass	10:31am

CRC Tests

Test	Status	Time
COMP	Pass	10:32am
CAL	Pass	10:32am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Moore Co. Instrument Location Southern Pines P.D.

Instrument Serial No. 008120 Southern Pines, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th **day of** March, **20** 20**, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

MOORE COUNTY SOUTHERN PINES PD 620

Serial Number: *008720*
Test Date: *03/25/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911501
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	6:12pm
AIR BLK	.00	6:12pm
ACCY CHK	.07	6:13pm
AIR BLK	.00	6:14pm
SUB TEST	.00	6:14pm
AIR BLK	.00	6:15pm
SUB TEST	.00	6:17pm
AIR BLK	.00	6:18pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MOORE COUNTY SOUTHERN PINES PD 620

Serial Number: *008720* Test Record Number: *1151*
Test Date: *03/25/2020* Test Time: *6:18pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:18pm
FLO	Pass	6:18pm
FC	Pass	6:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:19pm
SRC	Pass	6:19pm
DET	Pass	6:19pm
BAR	Pass	6:19pm
BT	Pass	6:19pm

Blank Tests

Test	Status	Time
AIR	Pass	6:19pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:19pm

CRC Tests

Test	Status	Time
COMP	Pass	6:20pm
CAL	Pass	6:20pm

Preventive Maintenance Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Moore Co. Instrument Location Moore Co. Detention Center

Instrument Serial No. D8735 Carthage, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th **day of** March, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

454
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

MOORE COUNTY DETENTION CENTER 620

Serial Number: *008735*
Test Date: *03/25/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911501
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	7:03pm
AIR BLK	.00	7:03pm
ACCY CHK	.08	7:04pm
AIR BLK	.00	7:05pm
SUB TEST	**.00**	**7:06pm**
AIR BLK	.00	7:07pm
SUB TEST	**.00**	**7:08pm**
AIR BLK	.00	7:09pm

Reported Average: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MOORE COUNTY DETENTION CENTER 620

Serial Number: *008735* Test Record Number: *2407*
Test Date: *03/25/2020* Test Time: *7:10pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:10pm
FLO	Pass	7:10pm
FC	Pass	7:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:10pm
SRC	Pass	7:10pm
DET	Pass	7:10pm
BAR	Pass	7:10pm
BT	Pass	7:10pm

Blank Tests

Test	Status	Time
AIR	Pass	7:11pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:11pm

CRC Tests

Test	Status	Time
COMP	Pass	7:11pm
CAL	Pass	7:11pm

Preventive Maintenance Status: Pass

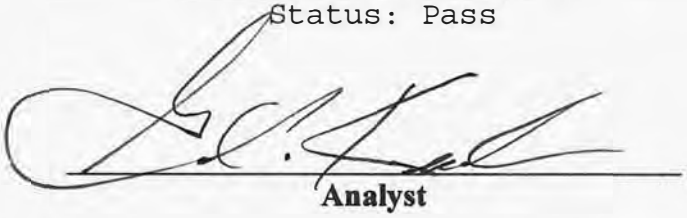

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County NEW HANOVER Instrument Location CAROLINA BEACH POLICE DEPT

Instrument Serial No. 008661

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 **day of** MARCH, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY CAROLINA BEACH PD
640

Serial Number: *008661*
Test Date: *03/30/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, ALVIN R*
Permit Number: *15671E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919902
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	10:19am
AIR BLK	.00	10:20am
ACCY CHK	.08	10:21am
AIR BLK	.00	10:22am
SUB TEST	**.00**	**10:22am**
AIR BLK	.00	10:23am
SUB TEST	**.00**	**10:24am**
AIR BLK	.00	10:25am

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY CAROLINA BEACH PD 640

Serial Number: *008661* Test Record Number: *2642*
Test Date: *03/30/2020* Test Time: *10:26am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:26am
FLO	Pass	10:26am
FC	Pass	10:26am

Temperature Tests

Test	Status	Time
FC1	Pass	10:27am
SRC	Pass	10:27am
DET	Pass	10:27am
BAR	Pass	10:27am
BT	Pass	10:27am

Blank Tests

Test	Status	Time
AIR	Pass	10:27am

Printer Tests

Test	Status	Time
PRNT	Pass	10:27am

CRC Tests

Test	Status	Time
COMP	Pass	10:27am
CAL	Pass	10:27am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Onslow Instrument Location Bat Mobile Unit 12

Instrument Serial No. 008600 Jacksonville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

665
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE 12 660

Serial Number: *008600*
Test Date: *03/13/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Anderson, Mark G*
Permit Number: *0013-1517*
Effective:
09/23/2019-09/23/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919902
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	10:19pm
AIR BLK	.00	10:20pm
ACCY CHK	.08	10:20pm
AIR BLK	.00	10:21pm
SUB TEST	**.00**	**10:22pm**
AIR BLK	.00	10:23pm
SUB TEST	**.00**	**10:24pm**
AIR BLK	.00	10:25pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE 12 660

Serial Number: *008600* Test Record Number: *1958*
Test Date: *03/13/2020* Test Time: *10:30pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:31pm
FLO	Pass	10:31pm
FC	Pass	10:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:31pm
SRC	Pass	10:31pm
DET	Pass	10:31pm
BAR	Pass	10:31pm
BT	Pass	10:31pm

Blank Tests

Test	Status	Time
AIR	Pass	10:31pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:31pm

CRC Tests

Test	Status	Time
COMP	Pass	10:32pm
CAL	Pass	10:32pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Onslow Instrument Location Bat Mobile Unit 12

Instrument Serial No. 008688 Jacksonville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

665
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE 12 660

Serial Number: *008698*
Test Date: *03/15/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Anderson, Mark G*
Permit Number: *0013-1517*
Effective:
09/23/2019-09/23/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG814901
Exp Date: 05/29/2020

Test	g/210L	Time
DIAG	Pass	2:32am
AIR BLK	.00	2:33am
ACCY CHK	.08	2:34am
AIR BLK	.00	2:35am
SUB TEST	**.00**	**2:35am**
AIR BLK	.00	2:36am
SUB TEST	**.00**	**2:38am**
AIR BLK	.00	2:39am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE 12 660

Serial Number: *008698* Test Record Number: *1527*
Test Date: *03/15/2020* Test Time: *2:40am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:40am
FLO	Pass	2:40am
FC	Pass	2:40am

Temperature Tests

Test	Status	Time
FC1	Pass	2:40am
SRC	Pass	2:40am
DET	Pass	2:40am
BAR	Pass	2:40am
BT	Pass	2:40am

Blank Tests

Test	Status	Time
AIR	Pass	2:41am

Printer Tests

Test	Status	Time
PRNT	Pass	2:41am

CRC Tests

Test	Status	Time
COMP	Pass	2:41am
CAL	Pass	2:41am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Onslow Instrument Location Bat Mobile Unit 12

Instrument Serial No. 008698 Jacksonville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

665
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE 12 660

Serial Number: *008698*
Test Date: *03/13/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Anderson, Mark G*
Permit Number: *0013-1517*
Effective:
09/23/2019-09/23/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG814901
Exp Date: 05/29/2020

Test	g/210L	Time
DIAG	Pass	10:16pm
AIR BLK	.00	10:17pm
ACCY CHK	.08	10:18pm
AIR BLK	.00	10:19pm
SUB TEST	**.00**	**10:19pm**
AIR BLK	.00	10:20pm
SUB TEST	**.00**	**10:22pm**
AIR BLK	.00	10:23pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE 12 660

Serial Number: *008698* Test Record Number: *1524*
Test Date: *03/13/2020* Test Time: *10:24pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:25pm
FLO	Pass	10:25pm
FC	Pass	10:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:25pm
SRC	Pass	10:25pm
DET	Pass	10:25pm
BAR	Pass	10:25pm
BT	Pass	10:25pm

Blank Tests

Test	Status	Time
AIR	Pass	10:26pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:26pm

CRC Tests

Test	Status	Time
COMP	Pass	10:26pm
CAL	Pass	10:26pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Onslow Instrument Location Bat mobile Unit 12

Instrument Serial No. 005698 Jacksonville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

665
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE 12 660

Serial Number: *008698*
Test Date: *03/11/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Anderson, Mark G*
Permit Number: *0013-1517*
Effective:
09/23/2019-09/23/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG814901
Exp Date: 05/29/2020

Test	g/210L	Time
DIAG	Pass	9:06pm
AIR BLK	.00	9:07pm
ACCY CHK	.07	9:07pm
AIR BLK	.00	9:08pm
SUB TEST	**.00**	**9:09pm**
AIR BLK	.00	9:10pm
SUB TEST	**.00**	**9:11pm**
AIR BLK	.00	9:12pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE 12 660

Serial Number: *008698* Test Record Number: *1521*
Test Date: *03/11/2020* Test Time: *9:22pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:23pm
FLO	Pass	9:23pm
FC	Pass	9:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:23pm
SRC	Pass	9:23pm
DET	Pass	9:23pm
BAR	Pass	9:23pm
BT	Pass	9:23pm

Blank Tests

Test	Status	Time
AIR	Pass	9:23pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:24pm

CRC Tests

Test	Status	Time
COMP	Pass	9:24pm
CAL	Pass	9:24pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Onslow Instrument Location Bat Mobile Unit 12

Instrument Serial No. 008788 Jacksonville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

665
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intoxilyzer EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE UNIT 12 660

Serial Number: *008788*
Test Date: *03/12/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Anderson, Mark G*
Permit Number: *0013-1517*
Effective:
09/23/2019-09/23/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911506
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	10:20pm
AIR BLK	.00	10:21pm
ACCY CHK	.08	10:22pm
AIR BLK	.00	10:23pm
SUB TEST	**.00**	**10:24pm**
AIR BLK	.00	10:24pm
SUB TEST	**.00**	**10:26pm**
AIR BLK	.00	10:27pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE UNIT 12 660

Serial Number: *008788* Test Record Number: *1504*
Test Date: *03/12/2020* Test Time: *10:31pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:31pm
FLO	Pass	10:31pm
FC	Pass	10:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:32pm
SRC	Pass	10:32pm
DET	Pass	10:32pm
BAR	Pass	10:32pm
BT	Pass	10:32pm

Blank Tests

Test	Status	Time
AIR	Pass	10:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:32pm

CRC Tests

Test	Status	Time
COMP	Pass	10:32pm
CAL	Pass	10:32pm

Preventive Maintenance
Status: Pass

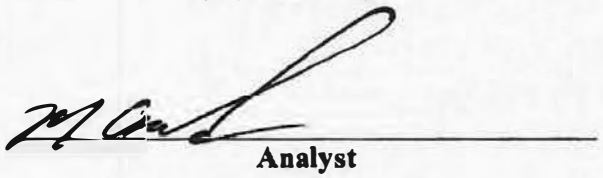

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Onslow Instrument Location Bat Mobile Unit 12

Instrument Serial No. 008788 Jacksonville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of March, 2023, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

665
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE UNIT 12 660

Serial Number: *008788*
Test Date: *03/14/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Anderson, Mark G*
Permit Number: *0013-1517*
Effective:
09/23/2019-09/23/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911506
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	10:43pm
AIR BLK	.00	10:44pm
ACCY CHK	.08	10:44pm
AIR BLK	.00	10:45pm
SUB TEST	**.00**	**10:46pm**
AIR BLK	.00	10:47pm
SUB TEST	**.00**	**10:48pm**
AIR BLK	.00	10:49pm

Reported AC .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE UNIT 12 660

Serial Number: *008788* Test Record Number: *1510*
Test Date: *03/14/2020* Test Time: *10:50pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:50pm
FLO	Pass	10:50pm
FC	Pass	10:50pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:51pm
SRC	Pass	10:51pm
DET	Pass	10:51pm
BAR	Pass	10:51pm
BT	Pass	10:51pm

Blank Tests

Test	Status	Time
AIR	Pass	10:51pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:51pm

CRC Tests

Test	Status	Time
COMP	Pass	10:51pm
CAL	Pass	10:51pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Onslow Instrument Location Bat Mobile Unit 12

Instrument Serial No. 008788 Jacksonville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of March, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

665
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE UNIT 12 660

Serial Number: *008788*
Test Date: *03/13/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Anderson, Mark G*
Permit Number: *0013-1517*
Effective:
09/23/2019-09/23/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911506
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	10:21pm
AIR BLK	.00	10:22pm
ACCY CHK	.08	10:23pm
AIR BLK	.00	10:24pm
SUB TEST	**.00**	**10:24pm**
AIR BLK	.00	10:25pm
SUB TEST	**.00**	**10:27pm**
AIR BLK	.00	10:28pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE UNIT 12 660

Serial Number: *008788* Test Record Number: *1507*
Test Date: *03/13/2020* Test Time: *10:31pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:31pm
FLO	Pass	10:31pm
FC	Pass	10:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:31pm
SRC	Pass	10:31pm
DET	Pass	10:31pm
BAR	Pass	10:31pm
BT	Pass	10:31pm

Blank Tests

Test	Status	Time
AIR	Pass	10:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:32pm

CRC Tests

Test	Status	Time
COMP	Pass	10:32pm
CAL	Pass	10:32pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County ONSLOW Instrument Location JACKSONVILLE

Instrument Serial No. 000930 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 **day of** MARCH **, 20** 20**, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Alan Ray Barnes
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

ONSLOW COUNTY JACKSONVILLE PD 660

Serial Number: *008930*
Test Date: *03/30/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, ALVIN R*
Permit Number: *15671E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG831801
Exp Date: 11/14/2020

Test	g/210L	Time
DIAG	Pass	12:41pm
AIR BLK	.00	12:42pm
ACCY CHK	.08	12:42pm
AIR BLK	.00	12:44pm
SUB TEST	**.00**	**12:44pm**
AIR BLK	.00	12:45pm
SUB TEST	**.00**	**12:46pm**
AIR BLK	.00	12:47pm

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

Calvin Ray Barnes
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY JACKSONVILLE PD 660

Serial Number: *008930* Test Record Number: *2072*
Test Date: *03/30/2020* Test Time: *12:50pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:51pm
FLO	Pass	12:51pm
FC	Pass	12:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:51pm
SRC	Pass	12:51pm
DET	Pass	12:51pm
BAR	Pass	12:51pm
BT	Pass	12:51pm

Blank Tests

Test	Status	Time
AIR	Pass	12:51pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:51pm

CRC Tests

Test	Status	Time
COMP	Pass	12:52pm
CAL	Pass	12:52pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County ORANGE Instrument Location Chapel H.11 PD

Instrument Serial No. 008839 828 Martin Luther King Jr BLVD
Chapel H.11, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of MARCH, 20 20 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ORANGE COUNTY CHAPEL HILL PD 670

Serial Number: *008839*
Test Date: *03/26/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, STOKES*
Permit Number: *11434E*
Effective:
04/01/2019-04/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911506
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	11:52am
AIR BLK	.00	11:52am
ACCY CHK	.08	11:53am
AIR BLK	.00	11:54am
SUB TEST	**.00**	**11:55am**
AIR BLK	.00	11:56am
SUB TEST	**.00**	**11:57am**
AIR BLK	.00	11:58am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ORANGE COUNTY CHAPEL HILL PD 670

Serial Number: *008839* Test Record Number: *2164*
Test Date: *03/26/2020* Test Time: *11:58am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:59am
FLO	Pass	11:59am
FC	Pass	11:59am

Temperature Tests

Test	Status	Time
FC1	Pass	11:59am
SRC	Pass	11:59am
DET	Pass	11:59am
BAR	Pass	11:59am
BT	Pass	11:59am

Blank Tests

Test	Status	Time
AIR	Pass	12:00pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:00pm

CRC Tests

Test	Status	Time
COMP	Pass	12:00pm
CAL	Pass	12:00pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County PAMLICO Instrument Location PAMLICO COUNTY

Instrument Serial No. 008640 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 **day of** MARCH **, 20** 20**, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA
MAY 20, 1775
APR. 12, 1776
ESSE QUAM VIDERI

Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PAMLICO COUNTY DETENTION CENTER 680

Serial Number: *008640*
Test Date: *03/24/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, ALVIN R*
Permit Number: *15671E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG934001
Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	1:46pm
AIR BLK	.00	1:47pm
ACCY CHK	.08	1:47pm
AIR BLK	.00	1:48pm
SUB TEST	**.00**	**1:50pm**
AIR BLK	.00	1:51pm
SUB TEST	**.00**	**1:53pm**
AIR BLK	.00	1:53pm

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

_____
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PAMLICO COUNTY DETENTION CENTER 680

Serial Number: *008640* Test Record Number: *1400*
Test Date: *03/24/2020* Test Time: *1:54pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:54pm
FLO	Pass	1:54pm
FC	Pass	1:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:54pm
SRC	Pass	1:54pm
DET	Pass	1:54pm
BAR	Pass	1:54pm
BT	Pass	1:54pm

Blank Tests

Test	Status	Time
AIR	Pass	1:55pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:55pm

CRC Tests

Test	Status	Time
COMP	Pass	1:55pm
CAL	Pass	1:55pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Pitt Instrument Location Pitt Co. Detention Center

Instrument Serial No. 008668 124 Detention Dr., Greenville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th **day of** March, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: *008668*
Test Date: *03/17/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *GUARD, KELLY G*
Permit Number: *12955E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG920301
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	10:32am
AIR BLK	.00	10:33am
ACCY CHK	.08	10:34am
AIR BLK	.00	10:35am
SUB TEST	**.00**	**10:36am**
AIR BLK	.00	10:37am
SUB TEST	**.00**	**10:38am**
AIR BLK	.00	10:39am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: *008668* Test Record Number: *3554*
Test Date: *03/17/2020* Test Time: *10:40am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:40am
FLO	Pass	10:40am
FC	Pass	10:40am

Temperature Tests

Test	Status	Time
FC1	Pass	10:40am
SRC	Pass	10:40am
DET	Pass	10:40am
BAR	Pass	10:40am
BT	Pass	10:40am

Blank Tests

Test	Status	Time
AIR	Pass	10:41am

Printer Tests

Test	Status	Time
PRNT	Pass	10:41am

CRC Tests

Test	Status	Time
COMP	Pass	10:41am
CAL	Pass	10:41am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Randolph Co. Instrument Location Randleman Police Dept.

Instrument Serial No. 008137 Randleman, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th **day of** March **, 20**20**, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY RANDLEMAN PD 750

Serial Number: *008737*
Test Date: *03/25/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG934001
Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	12:27pm
AIR BLK	.00	12:27pm
ACCY CHK	.08	12:28pm
AIR BLK	.00	12:29pm
SUB TEST	**.00**	**12:29pm**
AIR BLK	.00	12:30pm
SUB TEST	**.00**	**12:32pm**
AIR BLK	.00	12:33pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY RANDLEMAN PD 750

Serial Number: *008737* Test Record Number: *1157*
Test Date: *03/25/2020* Test Time: *12:33pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:33pm
FLO	Pass	12:33pm
FC	Pass	12:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:33pm
SRC	Pass	12:33pm
DET	Pass	12:33pm
BAR	Pass	12:33pm
BT	Pass	12:33pm

Blank Tests

Test	Status	Time
AIR	Pass	12:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:34pm

CRC Tests

Test	Status	Time
COMP	Pass	12:34pm
CAL	Pass	12:34pm

Preventive Maintenance
Status: Pass

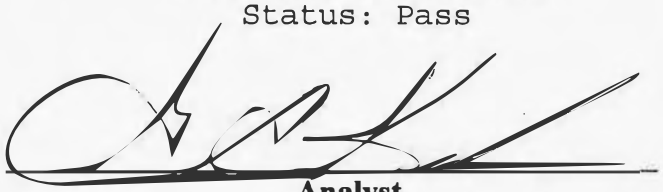

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Randolph Co. Instrument Location Liberty Police Dept

Instrument Serial No. 008830 Liberty P.D.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th **day of** March, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY LIBERTY PD 750

Serial Number: *008830*
Test Date: *03/25/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG934001
Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	11:27am
AIR BLK	.00	11:27am
ACCY CHK	.08	11:28am
AIR BLK	.00	11:29am
SUB TEST	**.00**	**11:30am**
AIR BLK	.00	11:30am
SUB TEST	**.00**	**11:32am**
AIR BLK	.00	11:33am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY LIBERTY PD 750

Serial Number: *008830* Test Record Number: *666*
Test Date: *03/25/2020* Test Time: *11:34am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:34am
FLO	Pass	11:34am
FC	Pass	11:34am

Temperature Tests

Test	Status	Time
FC1	Pass	11:34am
SRC	Pass	11:34am
DET	Pass	11:34am
BAR	Pass	11:34am
BT	Pass	11:34am

Blank Tests

Test	Status	Time
AIR	Pass	11:35am

Printer Tests

Test	Status	Time
PRNT	Pass	11:35am

CRC Tests

Test	Status	Time
COMP	Pass	11:35am
CAL	Pass	11:35am

Preventive Maintenance Status: Pass

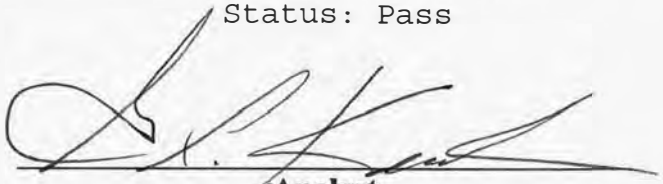

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Randolph Co. Instrument Location Randolph Co. Detention Center

Instrument Serial No. 008860 Asheboro NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th **day of** March, 2020, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY DETENTION CENTER 750

Serial Number: *008860*
Test Date: *03/25/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG902202
Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	2:06pm
AIR BLK	.00	2:07pm
ACCY CHK	.08	2:07pm
AIR BLK	.00	2:08pm
SUB TEST	**.00**	**2:09pm**
AIR BLK	.00	2:10pm
SUB TEST	**.00**	**2:11pm**
AIR BLK	.00	2:12pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY DETENTION CENTER 750

Serial Number: *008860* Test Record Number: *2794*
Test Date: *03/25/2020* Test Time: *2:13pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:13pm
FLO	Pass	2:13pm
FC	Pass	2:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:13pm
SRC	Pass	2:13pm
DET	Pass	2:13pm
BAR	Pass	2:13pm
BT	Pass	2:13pm

Blank Tests

Test	Status	Time
AIR	Pass	2:14pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:14pm

CRC Tests

Test	Status	Time
COMP	Pass	2:14pm
CAL	Pass	2:14pm

Preventive Maintenance Status: Pass

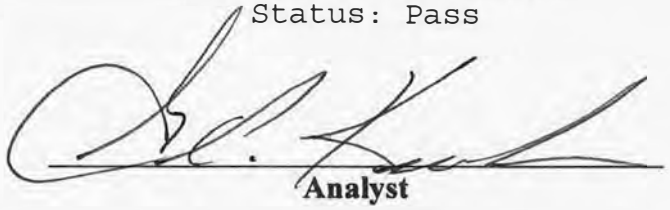

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Randolph Co. Instrument Location Randolph Co. Detention Center

Instrument Serial No. 008879 Asheboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th **day of** March, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY DETENTION CENTER 750

Serial Number: *008899*
Test Date: *03/25/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG902202
Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	1:40pm
AIR BLK	.00	1:41pm
ACCY CHK	.08	1:41pm
AIR BLK	.00	1:42pm
SUB TEST	**.00**	**1:43pm**
AIR BLK	.00	1:44pm
SUB TEST	**.00**	**1:45pm**
AIR BLK	.00	1:46pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY DETENTION CENTER 750

Serial Number: *008899* Test Record Number: *3376*
Test Date: *03/25/2020* Test Time: *1:47pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:47pm
FLO	Pass	1:47pm
FC	Pass	1:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:47pm
SRC	Pass	1:47pm
DET	Pass	1:47pm
BAR	Pass	1:47pm
BT	Pass	1:47pm

Blank Tests

Test	Status	Time
AIR	Pass	1:48pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:48pm

CRC Tests

Test	Status	Time
COMP	Pass	1:48pm
CAL	Pass	1:48pm

Preventive Maintenance Status: Pass

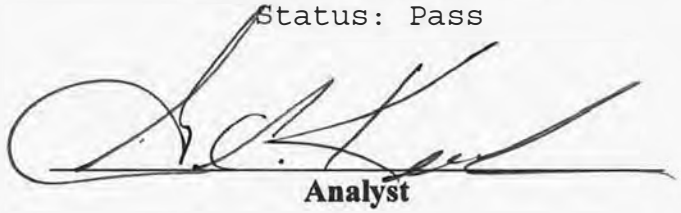

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Robeson Instrument Location BAT Mobile Unit #5

Instrument Serial No. 008616 Robeson County Sheriff's Dept.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of March, 20 20 the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: *008616*
Test Date: *03/07/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *TODD, SHANE C*
Permit Number: *11391E*
Effective:
07/27/2018-07/01/2020

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG933703
Exp Date: 03/12/2021

Test	g/210L	Time
DIAG	Pass	8:45pm
AIR BLK	.00	8:46pm
ACCY CHK	.08	8:46pm
AIR BLK	.00	8:47pm
SUB TEST	**.00**	**8:48pm**
AIR BLK	.00	8:48pm
SUB TEST	**.00**	**8:50pm**
AIR BLK	.00	8:51pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: *008616* Test Record Number: *2547*
Test Date: *03/07/2020* Test Time: *8:52pm EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:52pm
FLO	Pass	8:52pm
FC	Pass	8:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:52pm
SRC	Pass	8:52pm
DET	Pass	8:52pm
BAR	Pass	8:52pm
BT	Pass	8:52pm

Blank Tests

Test	Status	Time
AIR	Pass	8:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:53pm

CRC Tests

Test	Status	Time
COMP	Pass	8:53pm
CAL	Pass	8:53pm

Preventive Maintenance
Status: Pass

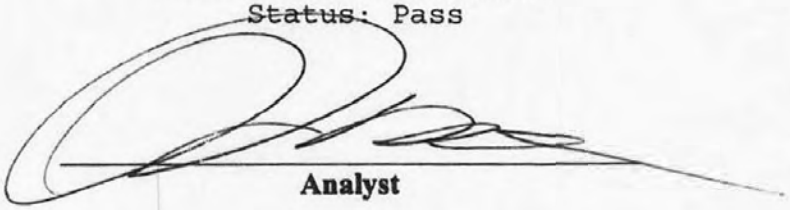

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Robeson Co. Instrument Location Lumberton Police Dept.

Instrument Serial No. 008629 Lumberton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24th day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

ROBESON COUNTY LUMBERTON PD 770

Serial Number: *008629*
Test Date: *03/24/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911506
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	10:50am
AIR BLK	.00	10:51am
ACCY CHK	.07	10:51am
AIR BLK	.00	10:52am
SUB TEST	**.00**	**10:53am**
AIR BLK	.00	10:54am
SUB TEST	**.00**	**10:56am**
AIR BLK	.00	10:56am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY LUMBERTON PD 770

Serial Number: *008629* Test Record Number: *862*
Test Date: *03/24/2020* Test Time: *10:57am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:58am
FLO	Pass	10:58am
FC	Pass	10:58am

Temperature Tests

Test	Status	Time
FC1	Pass	10:58am
SRC	Pass	10:58am
DET	Pass	10:58am
BAR	Pass	10:58am
BT	Pass	10:58am

Blank Tests

Test	Status	Time
AIR	Pass	10:58am

Printer Tests

Test	Status	Time
PRNT	Pass	10:58am

CRC Tests

Test	Status	Time
COMP	Pass	10:59am
CAL	Pass	10:59am

Preventive Maintenance
Status: Pass

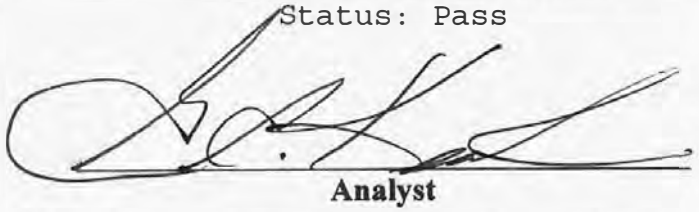

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Robeson Instrument Location BAT Mobile Unit #5

Instrument Serial No. 008704 Robeson County Sheriff's Dept.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of March, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: *008704*
Test Date: *03/07/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *TODD, SHANE C*
Permit Number: *11391E*
Effective:
07/27/2018-07/01/2020

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG807101
Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	8:43pm
AIR BLK	.00	8:44pm
ACCY CHK	.08	8:45pm
AIR BLK	.00	8:45pm
SUB TEST	**.00**	**8:47pm**
AIR BLK	.00	8:48pm
SUB TEST	**.00**	**8:49pm**
AIR BLK	.00	8:50pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: *008704* Test Record Number: *638*
Test Date: *03/07/2020* Test Time: *8:52pm EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:52pm
FLO	Pass	8:52pm
FC	Pass	8:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:52pm
SRC	Pass	8:52pm
DET	Pass	8:52pm
BAR	Pass	8:52pm
BT	Pass	8:52pm

Blank Tests

Test	Status	Time
AIR	Pass	8:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:53pm

CRC Tests

Test	Status	Time
COMP	Pass	8:53pm
CAL	Pass	8:53pm

Preventive Maintenance
Status: Pass

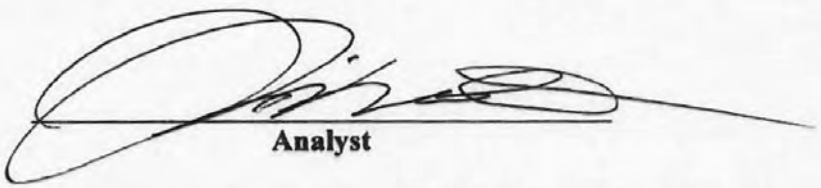

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Robeson Instrument Location BAT Mobile Unit #5

Instrument Serial No. 008707 Robeson Sheriff's Dept.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: *008707*
Test Date: *03/07/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *TODD, SHANE C*
Permit Number: *11391E*
Effective:
07/27/2018-07/01/2020

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919902
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	8:47pm
AIR BLK	.00	8:48pm
ACCY CHK	.08	8:48pm
AIR BLK	.00	8:49pm
SUB TEST	**.00**	**8:50pm**
AIR BLK	.00	8:51pm
SUB TEST	**.00**	**8:55pm**
AIR BLK	.00	8:56pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: *008707* Test Record Number: *2634*
Test Date: *03/07/2020* Test Time: *9:01pm EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:01pm
FLO	Pass	9:01pm
FC	Pass	9:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:01pm
SRC	Pass	9:01pm
DET	Pass	9:01pm
BAR	Pass	9:01pm
BT	Pass	9:01pm

Blank Tests

Test	Status	Time
AIR	Pass	9:02pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:02pm

CRC Tests

Test	Status	Time
COMP	Pass	9:02pm
CAL	Pass	9:02pm

Preventive Maintenance
Status: Pass

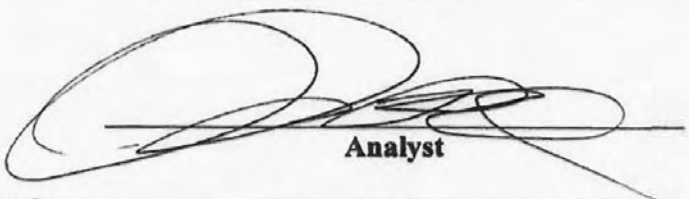

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Robeson Co. Instrument Location Robeson Co. Detention Center

Instrument Serial No. 008805 Lumberton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of March, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY DETENTION CENTER 770

Serial Number: *008805*
Test Date: *03/23/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG934001
Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	12:09pm
AIR BLK	.00	12:10pm
ACCY CHK	.08	12:10pm
AIR BLK	.00	12:12pm
SUB TEST	**.00**	**12:12pm**
AIR BLK	.00	12:13pm
SUB TEST	**.00**	**12:15pm**
AIR BLK	.00	12:16pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY DETENTION CENTER 770

Serial Number: *008805* Test Record Number: *4557*
Test Date: *03/23/2020* Test Time: *12:17pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:18pm
FLO	Pass	12:18pm
FC	Pass	12:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:18pm
SRC	Pass	12:18pm
DET	Pass	12:18pm
BAR	Pass	12:18pm
BT	Pass	12:18pm

Blank Tests

Test	Status	Time
AIR	Pass	12:18pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:18pm

CRC Tests

Test	Status	Time
COMP	Pass	12:19pm
CAL	Pass	12:19pm

Preventive Maintenance
Status: Pass

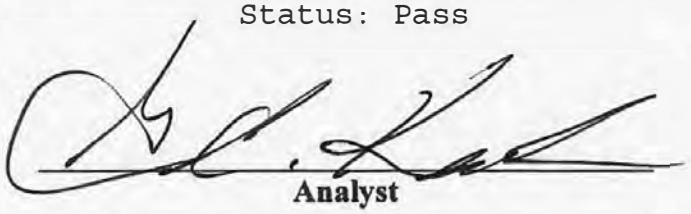

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Robeson Co. Instrument Location Robeson Co. Detention Center

Instrument Serial No. 018836 Lumberton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of March, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY DETENTION CENTER 770

Serial Number: *008836*
Test Date: *03/23/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Grayham C*
Permit Number: *0045-5487*
Effective:
11/04/2019-11/04/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG934001
Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	11:54am
AIR BLK	.00	11:55am
ACCY CHK	.08	11:56am
AIR BLK	.00	11:57am
SUB TEST	**.00**	**11:57am**
AIR BLK	.00	11:58am
SUB TEST	**.00**	**12:00pm**
AIR BLK	.00	12:00pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY DETENTION CENTER 770

Serial Number: *008836* Test Record Number: *5420*
Test Date: *03/23/2020* Test Time: *12:02pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:03pm
FLO	Pass	12:03pm
FC	Pass	12:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:03pm
SRC	Pass	12:03pm
DET	Pass	12:03pm
BAR	Pass	12:03pm
BT	Pass	12:03pm

Blank Tests

Test	Status	Time
AIR	Pass	12:03pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:04pm

CRC Tests

Test	Status	Time
COMP	Pass	12:04pm
CAL	Pass	12:04pm

Preventive Maintenance Status: Pass

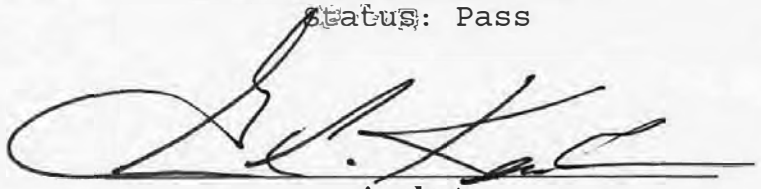

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Rockingham Instrument Location Eden PD

Instrument Serial No. D09636 Eden, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY EDEN PD 780

Serial Number: *008636*
Test Date: *03/04/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BURNETTE, ANTHONY J*
Permit Number: *11304E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911506
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	6:25pm
AIR BLK	.00	6:26pm
ACCY CHK	.08	6:27pm
AIR BLK	.00	6:28pm
SUB TEST	**.00**	**6:29pm**
AIR BLK	.00	6:30pm
SUB TEST	**.00**	**6:32pm**
AIR BLK	.00	6:33pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

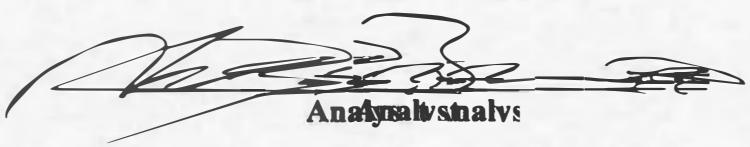

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY EDEN PD 780

Serial Number: *008636* Test Record Number: *2044*
Test Date: *03/04/2020* Test Time: *6:35pm EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:35pm
FLO	Pass	6:35pm
FC	Pass	6:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:35pm
SRC	Pass	6:35pm
DET	Pass	6:35pm
BAR	Pass	6:35pm
BT	Pass	6:35pm

Blank Tests

Test	Status	Time
AIR	Pass	6:36pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:36pm

CRC Tests

Test	Status	Time
COMP	Pass	6:36pm
CAL	Pass	6:36pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Rockingham Instrument Location Reidsville PD

Instrument Serial No. 008784 Reidsville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official — 649 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY REIDSVILLE PD 780

Serial Number: *008784*
Test Date: *03/09/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BURNETTE, ANTHONY J*
Permit Number: *11304E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911506
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	7:34pm
AIR BLK	.00	7:35pm
ACCY CHK	.08	7:35pm
AIR BLK	.00	7:37pm
SUB TEST	**.00**	**7:37pm**
AIR BLK	.00	7:38pm
SUB TEST	**.00**	**7:39pm**
AIR BLK	.00	7:40pm

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY REIDSVILLE PD 780

Serial Number: *008784* Test Record Number: *1200*
Test Date: *03/09/2020* Test Time: *7:43pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:43pm
FLO	Pass	7:43pm
FC	Pass	7:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:43pm
SRC	Pass	7:43pm
DET	Pass	7:43pm
BAR	Pass	7:43pm
BT	Pass	7:43pm

Blank Tests

Test	Status	Time
AIR	Pass	7:44pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:44pm

CRC Tests

Test	Status	Time
COMP	Pass	7:44pm
CAL	Pass	7:44pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Rockingham Instrument Location Rockingham Co. Jail

Instrument Serial No. 008796 Westworth, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY ROCKINGHAM CO JAIL
780

Serial Number: *008796*
Test Date: *03/05/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BURNETTE, ANTHONY J*
Permit Number: *11304E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919901
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	5:29pm
AIR BLK	.00	5:30pm
ACCY CHK	.08	5:31pm
AIR BLK	.00	5:32pm
SUB TEST	**.00**	**5:33pm**
AIR BLK	.00	5:34pm
SUB TEST	**.00**	**5:35pm**
AIR BLK	.00	5:36pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY ROCKINGHAM CO JAIL 780

Serial Number: *008796* Test Record Number: *2951*
Test Date: *03/05/2020* Test Time: *5:37pm EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:37pm
FLO	Pass	5:37pm
FC	Pass	5:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:37pm
SRC	Pass	5:37pm
DET	Pass	5:37pm
BAR	Pass	5:37pm
BT	Pass	5:37pm

Blank Tests

Test	Status	Time
AIR	Pass	5:38pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:38pm

CRC Tests

Test	Status	Time
COMP	Pass	5:38pm
CAL	Pass	5:38pm

Preventive Maintenance
Status: Pass

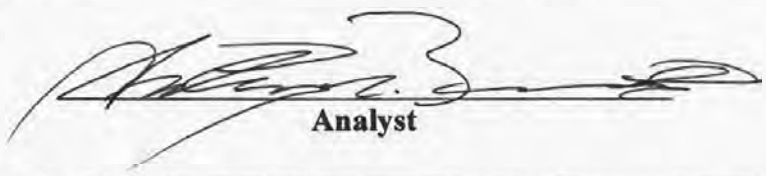

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Rockingham Instrument Location Madison PD

Instrument Serial No. CO98802 Madison, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of March, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY MADISON PD 780

Serial Number: *008802*
Test Date: *03/11/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BURNETTE, ANTHONY J*
Permit Number: *11304E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG831801
Exp Date: 11/14/2020

Test	g/210L	Time
DIAG	Pass	7:38pm
AIR BLK	.00	7:39pm
ACCY CHK	.08	7:40pm
AIR BLK	.00	7:41pm
SUB TEST	**.00**	**7:42pm**
AIR BLK	.00	7:42pm
SUB TEST	**.00**	**7:44pm**
AIR BLK	.00	7:45pm

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

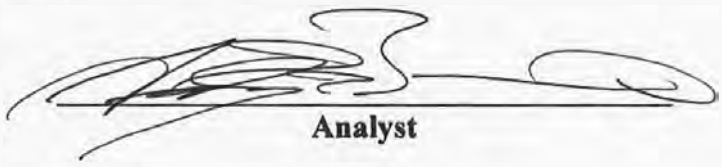

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY MADISON PD 780

Serial Number: *008802* Test Record Number: *863*
Test Date: *03/11/2020* Test Time: *7:46pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:46pm
FLO	Pass	7:46pm
FC	Pass	7:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:47pm
SRC	Pass	7:47pm
DET	Pass	7:47pm
BAR	Pass	7:47pm
BT	Pass	7:47pm

Blank Tests

Test	Status	Time
AIR	Pass	7:47pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:47pm

CRC Tests

Test	Status	Time
COMP	Pass	7:47pm
CAL	Pass	7:47pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Rutherford Instrument Location Forest City

Instrument Serial No. 008889 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 day of March, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

RUTHERFORD COUNTY FOREST CITY PD 800

Serial Number: *008889*
Test Date: *03/30/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Hays, Mark D*
Permit Number: *0011-3099*
Effective:
11/13/2019-11/13/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	9:52am
AIR BLK	.00	9:53am
ACCY CHK	.07	9:54am
AIR BLK	.00	9:55am
SUB TEST	**.00**	**9:56am**
AIR BLK	.00	9:57am
SUB TEST	**.00**	**9:58am**
AIR BLK	.00	9:59am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RUTHERFORD COUNTY FOREST CITY PD 800

Serial Number: *008889* Test Record Number: *887*
Test Date: *03/30/2020* Test Time: *10:01am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:01am
FLO	Pass	10:01am
FC	Pass	10:01am

Temperature Tests

Test	Status	Time
FC1	Pass	10:02am
SRC	Pass	10:02am
DET	Pass	10:02am
BAR	Pass	10:02am
BT	Pass	10:02am

Blank Tests

Test	Status	Time
AIR	Pass	10:02am

Printer Tests

Test	Status	Time
PRNT	Pass	10:02am

CRC Tests

Test	Status	Time
COMP	Pass	10:02am
CAL	Pass	10:02am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Rutherford Instrument Location Rutherford County Sheriffs Office

Instrument Serial No. 008914

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

RUTHERFORD COUNTY RUTHERFORD COUNTY SO 800

Serial Number: *008914*
Test Date: *03/30/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Hays, Mark D*
Permit Number: *0011-3099*
Effective:
11/13/2019-11/13/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG934303
Exp Date: 12/09/2021

Test	g/210L	Time
DIAG	Pass	8:57am
AIR BLK	.00	8:58am
ACCY CHK	.08	8:59am
AIR BLK	.00	9:00am
SUB TEST	**.00**	**9:00am**
AIR BLK	.00	9:01am
SUB TEST	**.00**	**9:03am**
AIR BLK	.00	9:04am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RUTHERFORD COUNTY RUTHERFORD COUNTY SO 800

Serial Number: *008914* Test Record Number: *2167*
Test Date: *03/30/2020* Test Time: *9:05am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:05am
FLO	Pass	9:05am
FC	Pass	9:06am

Temperature Tests

Test	Status	Time
FC1	Pass	9:06am
SRC	Pass	9:06am
DET	Pass	9:06am
BAR	Pass	9:06am
BT	Pass	9:06am

Blank Tests

Test	Status	Time
AIR	Pass	9:06am

Printer Tests

Test	Status	Time
PRNT	Pass	9:06am

CRC Tests

Test	Status	Time
COMP	Pass	9:06am
CAL	Pass	9:06am

Preventive Maintenance
Status: Pass

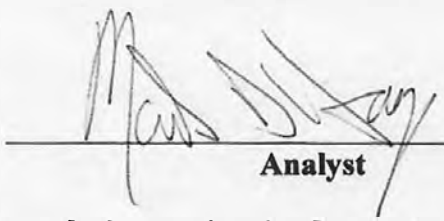

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Stokes Instrument Location Stokes Co Jail

Instrument Serial No. 005596 Danbury, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official — Certificate Number 649

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

STOKES COUNTY STOKES COUNTY JAIL 840

Serial Number: *008596*
Test Date: *03/10/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BURNETTE, ANTHONY J*
Permit Number: *11304E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG821801
Exp Date: 08/06/2020

Test	g/210L	Time
DIAG	Pass	7:52pm
AIR BLK	.00	7:53pm
ACCY CHK	.08	7:53pm
AIR BLK	.00	7:54pm
SUB TEST	**.00**	**7:55pm**
AIR BLK	.00	7:56pm
SUB TEST	**.00**	**7:57pm**
AIR BLK	.00	7:58pm

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

STOKES COUNTY STOKES COUNTY JAIL 840

Serial Number: *008596* Test Record Number: *1130*
Test Date: *03/10/2020* Test Time: *7:59pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:00pm
FLO	Pass	8:00pm
FC	Pass	8:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:00pm
SRC	Pass	8:00pm
DET	Pass	8:00pm
BAR	Pass	8:00pm
BT	Pass	8:00pm

Blank Tests

Test	Status	Time
AIR	Pass	8:01pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:01pm

CRC Tests

Test	Status	Time
COMP	Pass	8:01pm
CAL	Pass	8:01pm

Preventive Maintenance
Status: Pass

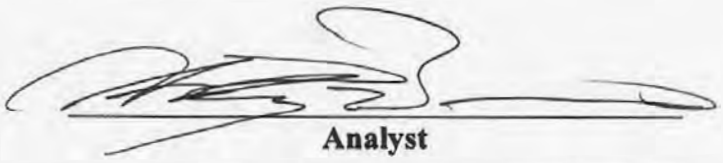

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Surry Instrument Location Surry County Jail

Instrument Serial No. 008934 Dobson, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of March, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

657
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

SURRY COUNTY SURRY CO JAIL 850

Serial Number: *008934*
Test Date: *03/27/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name:
BENFIELD II, KENNETH R
Permit Number: *22067E*
Effective:
06/01/2018-06/01/2020

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG821401
Exp Date: 08/02/2020

Test	g/210L	Time
DIAG	Pass	1:39pm
AIR BLK	.00	1:40pm
ACCY CHK	.07	1:40pm
AIR BLK	.00	1:41pm
SUB TEST	**.00**	**1:42pm**
AIR BLK	.00	1:43pm
SUB TEST	**.00**	**1:44pm**
AIR BLK	.00	1:45pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY SURRY CO JAIL 850

Serial Number: *008934* Test Record Number: *2115*
Test Date: *03/27/2020* Test Time: *1:46pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:46pm
FLO	Pass	1:46pm
FC	Pass	1:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:47pm
SRC	Pass	1:47pm
DET	Pass	1:47pm
BAR	Pass	1:47pm
BT	Pass	1:47pm

Blank Tests

Test	Status	Time
AIR	Pass	1:47pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:47pm

CRC Tests

Test	Status	Time
COMP	Pass	1:47pm
CAL	Pass	1:47pm

Preventive Maintenance Status: Pass

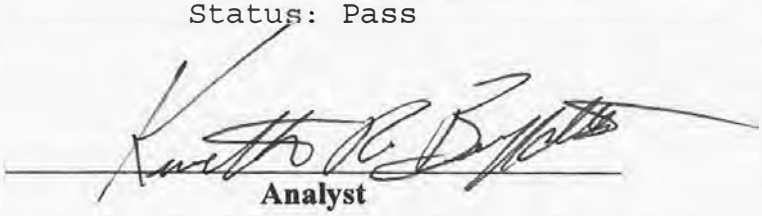

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Surry Instrument Location Pilot Mountain Police Department

Instrument Serial No. 008938

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

657
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SURRY COUNTY PILOT MOUNTAIN PD 850

Serial Number: *008938*
Test Date: *03/27/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name:
BENFIELD II, KENNETH R
Permit Number: *22067E*
Effective:
06/01/2018-06/01/2020

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919901
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	12:13pm
AIR BLK	.00	12:14pm
ACCY CHK	.08	12:15pm
AIR BLK	.00	12:16pm
SUB TEST	**.00**	**12:17pm**
AIR BLK	.00	12:18pm
SUB TEST	**.00**	**12:19pm**
AIR BLK	.00	12:20pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY PILOT MOUNTAIN PD 850

Serial Number: *008938* Test Record Number: *674*
Test Date: *03/27/2020* Test Time: *12:21pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:21pm
FLO	Pass	12:21pm
FC	Pass	12:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:22pm
SRC	Pass	12:22pm
DET	Pass	12:22pm
BAR	Pass	12:22pm
BT	Pass	12:22pm

Blank Tests

Test	Status	Time
AIR	Pass	12:22pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:22pm

CRC Tests

Test	Status	Time
COMP	Pass	12:22pm
CAL	Pass	12:22pm

Preventive Maintenance
Status: Pass

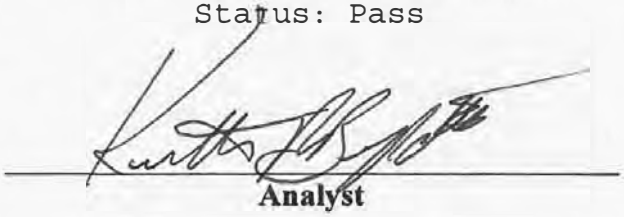

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Surry Instrument Location Mount Airy

Instrument Serial No. 008943 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

657
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

SURRY COUNTY MOUNT AIRY PD 850

Serial Number: *008943*
Test Date: *03/27/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name:
BENFIELD II, KENNETH R
Permit Number: *22067E*
Effective:
06/01/2018-06/01/2020

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG821401
Exp Date: 08/02/2020

Test	g/210L	Time
DIAG	Pass	12:56pm
AIR BLK	.00	12:57pm
ACCY CHK	.08	12:57pm
AIR BLK	.00	12:58pm
SUB TEST	**.00**	**12:59pm**
AIR BLK	.00	1:00pm
SUB TEST	**.00**	**1:01pm**
AIR BLK	.00	1:02pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY MOUNT AIRY PD 850

Serial Number: *008943* Test Record Number: *2191*
Test Date: *03/27/2020* Test Time: *1:03pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:03pm
FLO	Pass	1:03pm
FC	Pass	1:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:03pm
SRC	Pass	1:03pm
DET	Pass	1:03pm
BAR	Pass	1:03pm
BT	Pass	1:03pm

Blank Tests

Test	Status	Time
AIR	Pass	1:04pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:04pm

CRC Tests

Test	Status	Time
COMP	Pass	1:04pm
CAL	Pass	1:04pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Surry Instrument Location Elkin PD

Instrument Serial No. 008926 Elkin, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

SURRY COUNTY ELKIN PD 850

Serial Number: *008926*
Test Date: *03/27/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BURNETTE, ANTHONY J*
Permit Number: *11304E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG920301
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	3:38pm
AIR BLK	.00	3:38pm
ACCY CHK	.08	3:39pm
AIR BLK	.00	3:41pm
SUB TEST	**.00**	**3:41pm**
AIR BLK	.00	3:42pm
SUB TEST	**.00**	**3:44pm**
AIR BLK	.00	3:45pm

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY ELKIN PD 850

Serial Number: *008926* Test Record Number: *892*
Test Date: *03/27/2020* Test Time: *3:46pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:46pm
FLO	Pass	3:46pm
FC	Pass	3:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:46pm
SRC	Pass	3:46pm
DET	Pass	3:46pm
BAR	Pass	3:46pm
BT	Pass	3:46pm

Blank Tests

Test	Status	Time
AIR	Pass	3:47pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:47pm

CRC Tests

Test	Status	Time
COMP	Pass	3:47pm
CAL	Pass	3:47pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Swain Instrument Location Swain Co. Jail

Instrument Serial No. 008723 Bryson City, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

David R. Cuthrell — Signature of Certifying Official

635 — Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

SWAIN COUNTY SWAIN COUNTY JAIL 860

Serial Number: *008723*
Test Date: *03/09/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
07/12/2019-07/12/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG920301
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	1:43pm
AIR BLK	.00	1:44pm
ACCY CHK	.08	1:44pm
AIR BLK	.00	1:45pm
SUB TEST	**.00**	**1:46pm**
AIR BLK	.00	1:47pm
SUB TEST	**.00**	**1:48pm**
AIR BLK	.00	1:49pm

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SWAIN COUNTY SWAIN COUNTY JAIL 860

Serial Number: *008723* Test Record Number: *761*
Test Date: *03/09/2020* Test Time: *1:50pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:50pm
FLO	Pass	1:50pm
FC	Pass	1:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:51pm
SRC	Pass	1:51pm
DET	Pass	1:51pm
BAR	Pass	1:51pm
BT	Pass	1:51pm

Blank Tests

Test	Status	Time
AIR	Pass	1:51pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:51pm

CRC Tests

Test	Status	Time
COMP	Pass	1:52pm
CAL	Pass	1:52pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Swain Instrument Location Swain Co. Jail

Instrument Serial No. 008727 Bryson City, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th **day of** March, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SWAIN COUNTY SWAIN COUNTY JAIL 860

Serial Number: *008727*
Test Date: *03/09/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
07/12/2019-00/00/0000

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911506
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	1:44pm
AIR BLK	.00	1:45pm
ACCY CHK	.07	1:46pm
AIR BLK	.00	1:47pm
SUB TEST	**.00**	**1:47pm**
AIR BLK	.00	1:48pm
SUB TEST	**.00**	**1:50pm**
AIR BLK	.00	1:50pm

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SWAIN COUNTY SWAIN COUNTY JAIL 860

Serial Number: *008727* Test Record Number: *1332*
Test Date: *03/09/2020* Test Time: *1:52pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:52pm
FLO	Pass	1:52pm
FC	Pass	1:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:52pm
SRC	Pass	1:52pm
DET	Pass	1:52pm
BAR	Pass	1:52pm
BT	Pass	1:52pm

Blank Tests

Test	Status	Time
AIR	Pass	1:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:53pm

CRC Tests

Test	Status	Time
COMP	Pass	1:53pm
CAL	Pass	1:53pm

Preventive Maintenance
Status: Pass

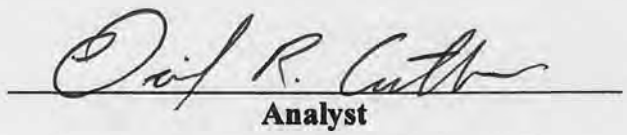

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Swain Instrument Location Cherokee Tribal Detention

Instrument Serial No. 008782 Cherokee, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of March, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

SWAIN COUNTY CHEROKEE DETENTION 860

Serial Number: *008782*
Test Date: *03/09/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
07/12/2019-07/12/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG920301
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	2:40pm
AIR BLK	.00	2:41pm
ACCY CHK	.08	2:41pm
AIR BLK	.00	2:42pm
SUB TEST	**.00**	**2:43pm**
AIR BLK	.00	2:44pm
SUB TEST	**.00**	**2:45pm**
AIR BLK	.00	2:46pm

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

_____
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SWAIN COUNTY CHEROKEE DETENTION 860

Serial Number: *008782* Test Record Number: *1171*
Test Date: *03/09/2020* Test Time: *2:47pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:47pm
FLO	Pass	2:47pm
FC	Pass	2:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:47pm
SRC	Pass	2:47pm
DET	Pass	2:47pm
BAR	Pass	2:47pm
BT	Pass	2:47pm

Blank Tests

Test	Status	Time
AIR	Pass	2:48pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:48pm

CRC Tests

Test	Status	Time
COMP	Pass	2:48pm
CAL	Pass	2:48pm

Preventive Maintenance
Status: Pass

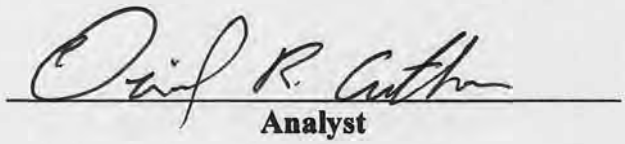

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Transylvania Instrument Location Transylvania Co. Jail

Instrument Serial No. 008609 Brevard, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of March, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

David R. Cutler — Signature of Certifying Official

635 — Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

TRANSYLVANIA COUNTY TRANSYLVANIA CO
JAIL 870

Serial Number: *008609*
Test Date: *03/16/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
07/12/2019-07/12/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG920301
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	11:18am
AIR BLK	.00	11:19am
ACCY CHK	.08	11:20am
AIR BLK	.00	11:21am
SUB TEST	**.00**	**11:22am**
AIR BLK	.00	11:22am
SUB TEST	**.00**	**11:24am**
AIR BLK	.00	11:25am

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

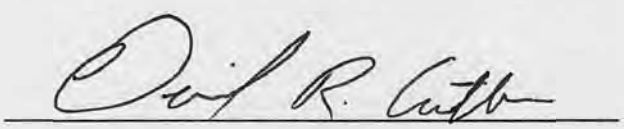

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

TRANSYLVANIA COUNTY TRANSYLVANIA CO JAIL 870

Serial Number: *008609* Test Record Number: *879*
Test Date: *03/16/2020* Test Time: *11:26am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:26am
FLO	Pass	11:26am
FC	Pass	11:26am

Temperature Tests

Test	Status	Time
FC1	Pass	11:26am
SRC	Pass	11:26am
DET	Pass	11:26am
BAR	Pass	11:26am
BT	Pass	11:26am

Blank Tests

Test	Status	Time
AIR	Pass	11:27am

Printer Tests

Test	Status	Time
PRNT	Pass	11:27am

CRC Tests

Test	Status	Time
COMP	Pass	11:27am
CAL	Pass	11:27am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Transylvania Instrument Location Transylvania Co. Jail

Instrument Serial No. 008820 Brevard, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of March, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

David R. Cutler — Signature of Certifying Official

635 — Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

TRANSYLVANIA COUNTY TRANSYLVANIA CO JAIL 870

Serial Number: *008820*
Test Date: *03/16/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
07/12/2019-07/12/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG920301
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	11:35am
AIR BLK	.00	11:36am
ACCY CHK	.07	11:37am
AIR BLK	.00	11:38am
SUB TEST	**.00**	**11:38am**
AIR BLK	.00	11:39am
SUB TEST	**.00**	**11:40am**
AIR BLK	.00	11:41am

Reported AC: .00 g/210L

_____
Signature of Chemical Analyst

Court CVR

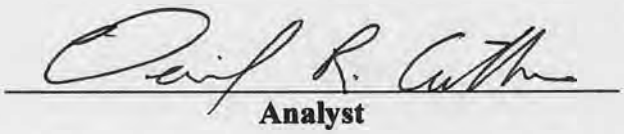

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

TRANSYLVANIA COUNTY TRANSYLVANIA CO JAIL 870

Serial Number: *008820* Test Record Number: *1309*
Test Date: *03/16/2020* Test Time: *11:42am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:42am
FLO	Pass	11:42am
FC	Pass	11:42am

Temperature Tests

Test	Status	Time
FC1	Pass	11:43am
SRC	Pass	11:43am
DET	Pass	11:43am
BAR	Pass	11:43am
BT	Pass	11:43am

Blank Tests

Test	Status	Time
AIR	Pass	11:43am

Printer Tests

Test	Status	Time
PRNT	Pass	11:43am

CRC Tests

Test	Status	Time
COMP	Pass	11:43am
CAL	Pass	11:43am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Union Instrument Location Waxhaw PD

Instrument Serial No. 008598 3620 Providence Rd, Waxhaw

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13th **day of** March, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Joseph C. Hutt
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

UNION COUNTY WAXHAW PD 890

Serial Number: *008598*
Test Date: *03/13/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Hutchinson, Joseph E*
Permit Number: *0035-6075*
Effective:
07/09/2019-07/09/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919901
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	3:25pm
AIR BLK	.00	3:26pm
ACCY CHK	.07	3:26pm
AIR BLK	.00	3:28pm
SUB TEST	**.00**	**3:28pm**
AIR BLK	.00	3:29pm
SUB TEST	**.00**	**3:31pm**
AIR BLK	.00	3:31pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY WAXHAW PD 890

Serial Number: *008598* Test Record Number: *833*
Test Date: *03/13/2020* Test Time: *3:32pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:33pm
FLO	Pass	3:33pm
FC	Pass	3:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:33pm
SRC	Pass	3:33pm
DET	Pass	3:33pm
BAR	Pass	3:33pm
BT	Pass	3:33pm

Blank Tests

Test	Status	Time
AIR	Pass	3:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:33pm

CRC Tests

Test	Status	Time
COMP	Pass	3:34pm
CAL	Pass	3:34pm

Preventive Maintenance
Status: Pass

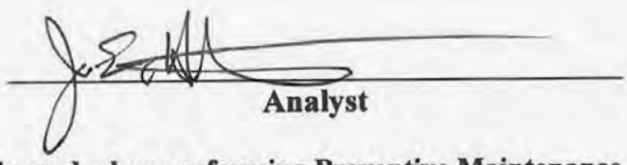

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Union Instrument Location Waxhaw PD

Instrument Serial No. 008598 3620 Providence Rd, Waxhaw

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13th **day of** March, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Joseph C. Hutt
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

UNION COUNTY WAXHAW PD 890

Serial Number: *008598*
Test Date: *03/13/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Hutchinson, Joseph E*
Permit Number: *0035-6075*
Effective:
07/09/2019-07/09/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919901
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	3:25pm
AIR BLK	.00	3:26pm
ACCY CHK	.07	3:26pm
AIR BLK	.00	3:28pm
SUB TEST	**.00**	**3:28pm**
AIR BLK	.00	3:29pm
SUB TEST	**.00**	**3:31pm**
AIR BLK	.00	3:31pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY WAXHAW PD 890

Serial Number: *008598* Test Record Number: *833*
Test Date: *03/13/2020* Test Time: *3:32pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:33pm
FLO	Pass	3:33pm
FC	Pass	3:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:33pm
SRC	Pass	3:33pm
DET	Pass	3:33pm
BAR	Pass	3:33pm
BT	Pass	3:33pm

Blank Tests

Test	Status	Time
AIR	Pass	3:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:33pm

CRC Tests

Test	Status	Time
COMP	Pass	3:34pm
CAL	Pass	3:34pm

Preventive Maintenance
Status: Pass

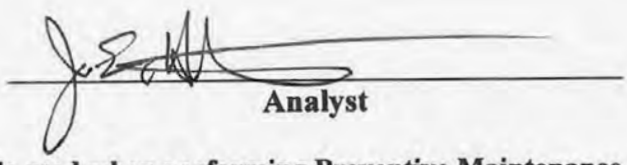

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County WAKE Instrument Location SAT MOBILE UNIT C

Instrument Serial No. 00 5570 CANON

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of MARCH, 20 20, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

443
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 6 910

Serial Number: *008580*
Test Date: *03/06/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Varnell, Bryon L*
Permit Number: *0036-1210*
Effective:
08/14/2019-08/14/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911506
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	6:37pm
AIR BLK	.00	6:38pm
ACCY CHK	.07	6:38pm
AIR BLK	.00	6:39pm
SUB TEST	**.00**	**6:40pm**
AIR BLK	.00	6:41pm
SUB TEST	**.00**	**6:42pm**
AIR BLK	.00	6:43pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 6 910

Serial Number: *008580* Test Record Number: *2554*
Test Date: *03/06/2020* Test Time: *6:45pm EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:45pm
FLO	Pass	6:45pm
FC	Pass	6:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:46pm
SRC	Pass	6:46pm
DET	Pass	6:46pm
BAR	Pass	6:46pm
BT	Pass	6:46pm

Blank Tests

Test	Status	Time
AIR	Pass	6:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:46pm

CRC Tests

Test	Status	Time
COMP	Pass	6:47pm
CAL	Pass	6:47pm

Preventive Maintenance
Status: Pass

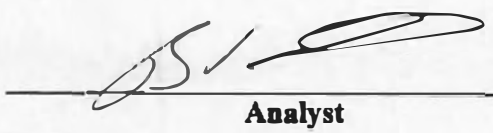

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County WAKE Instrument Location SAT MOBILE UNIT 6

Instrument Serial No. 605594 CANVAS

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of MARCH, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

663
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 6 910

Serial Number: *008584*
Test Date: *03/06/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Varnell, Bryon L*
Permit Number: *0036-1210*
Effective:
08/14/2019-08/14/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG902201
Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	6:37pm
AIR BLK	.00	6:38pm
ACCY CHK	.07	6:39pm
AIR BLK	.00	6:40pm
SUB TEST	**.00**	**6:40pm**
AIR BLK	.00	6:41pm
SUB TEST	**.00**	**6:43pm**
AIR BLK	.00	6:44pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 6 910

Serial Number: *008584* Test Record Number: *2319*
Test Date: *03/06/2020* Test Time: *6:46pm EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:46pm
FLO	Pass	6:46pm
FC	Pass	6:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:46pm
SRC	Pass	6:46pm
DET	Pass	6:46pm
BAR	Pass	6:46pm
BT	Pass	6:46pm

Blank Tests

Test	Status	Time
AIR	Pass	6:47pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:47pm

CRC Tests

Test	Status	Time
COMP	Pass	6:47pm
CAL	Pass	6:47pm

Preventive Maintenance
Status: Pass

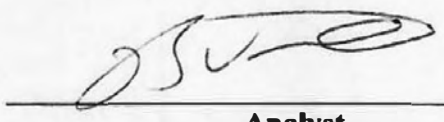

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County WAKE Instrument Location Raleigh PD NorthEast Dist

Instrument Serial No. 008623 5228 Green Dairy RD Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of MARCH, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY NORTH EAST DISTRICT 910

Serial Number: *008623*
Test Date: *03/10/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, STOKES*
Permit Number: *11434E*
Effective:
04/01/2019-04/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG902201
Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	2:41pm
AIR BLK	.00	2:42pm
ACCY CHK	.08	2:43pm
AIR BLK	.00	2:44pm
SUB TEST	**.00**	**2:44pm**
AIR BLK	.00	2:45pm
SUB TEST	**.00**	**2:47pm**
AIR BLK	.00	2:48pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY NORTH EAST DISTRICT 910

Serial Number: *008623* Test Record Number: *3976*
Test Date: *03/10/2020* Test Time: *2:49pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:50pm
FLO	Pass	2:50pm
FC	Pass	2:50pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:50pm
SRC	Pass	2:50pm
DET	Pass	2:50pm
BAR	Pass	2:50pm
BT	Pass	2:50pm

Blank Tests

Test	Status	Time
AIR	Pass	2:51pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:51pm

CRC Tests

Test	Status	Time
COMP	Pass	2:51pm
CAL	Pass	2:51pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County WAKE Instrument Location SAT MOBILE UNIT 6

Instrument Serial No. 007686 CARNEY

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of MARCH, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

663
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 6 910

Serial Number: *008686*
Test Date: *03/06/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Varnell, Bryon L*
Permit Number: *0036-1210*
Effective:
08/14/2019-08/14/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911506
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	6:36pm
AIR BLK	.00	6:37pm
ACCY CHK	.07	6:38pm
AIR BLK	.00	6:38pm
SUB TEST	**.00**	**6:39pm**
AIR BLK	.00	6:40pm
SUB TEST	**.00**	**6:41pm**
AIR BLK	.00	6:42pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 6 910

Serial Number: *008686* Test Record Number: *6680*
Test Date: *03/06/2020* Test Time: *6:43pm EST*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:44pm
FLO	Pass	6:44pm
FC	Pass	6:44pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:44pm
SRC	Pass	6:44pm
DET	Pass	6:44pm
BAR	Pass	6:44pm
BT	Pass	6:44pm

Blank Tests

Test	Status	Time
AIR	Pass	6:44pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:44pm

CRC Tests

Test	Status	Time
COMP	Pass	6:45pm
CAL	Pass	6:45pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County WAKE Instrument Location WAKE FOREST PD

Instrument Serial No. 008700 225 S. TAYLOR ST. WAKE FOREST, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of MARCH, 20 20 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

B L Smith
Signature of Certifying Official

637
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY WAKE FOREST PD 910

Serial Number: *008700*
Test Date: *03/10/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Smith, Brian D*
Permit Number: *0032-6608*
Effective:
07/09/2019-07/09/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG934303
Exp Date: 12/09/2021

Test	g/210L	Time
DIAG	Pass	5:00pm
AIR BLK	.00	5:00pm
ACCY CHK	.08	5:01pm
AIR BLK	.00	5:02pm
SUB TEST	**.00**	**5:03pm**
AIR BLK	.00	5:04pm
SUB TEST	**.00**	**5:05pm**
AIR BLK	.00	5:06pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY WAKE FOREST PD 910

Serial Number: *008700* Test Record Number: *1668*
Test Date: *03/10/2020* Test Time: *5:06pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:07pm
FLO	Pass	5:07pm
FC	Pass	5:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:07pm
SRC	Pass	5:07pm
DET	Pass	5:07pm
BAR	Pass	5:07pm
BT	Pass	5:07pm

Blank Tests

Test	Status	Time
AIR	Pass	5:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:08pm

CRC Tests

Test	Status	Time
COMP	Pass	5:08pm
CAL	Pass	5:08pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Wake Instrument Location Knightdale PD

Instrument Serial No. 008835 979 Steeple Square Ct. Knightdale, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of MARCH, 20 20 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY KNIGHTDALE PS 910

Serial Number: *008838*
Test Date: *03/10/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, STOKES*
Permit Number: *11434E*
Effective:
04/01/2019-04/01/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919902
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	1:06pm
AIR BLK	.00	1:07pm
ACCY CHK	.07	1:08pm
AIR BLK	.00	1:09pm
SUB TEST	**.00**	**1:09pm**
AIR BLK	.00	1:10pm
SUB TEST	**.00**	**1:12pm**
AIR BLK	.00	1:13pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY KNIGHTDALE PS 910

Serial Number: *008838* Test Record Number: *1981*
Test Date: *03/10/2020* Test Time: *1:14pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:14pm
FLO	Pass	1:14pm
FC	Pass	1:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:14pm
SRC	Pass	1:14pm
DET	Pass	1:14pm
BAR	Pass	1:14pm
BT	Pass	1:14pm

Blank Tests

Test	Status	Time
AIR	Pass	1:15pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:15pm

CRC Tests

Test	Status	Time
COMP	Pass	1:15pm
CAL	Pass	1:15pm

Preventive Maintenance
Status: Pass

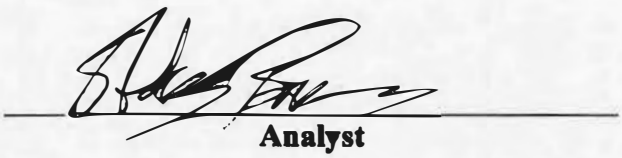

Analyst

This form is used ~~when performing Preventive~~ Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County WAYNE Instrument Location SAT MOBILE UNIT 6

Instrument Serial No. 008637 COLUMBUS

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of MARCH, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

443
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

WAYNE COUNTY BAT MOBILE UNIT 6 950

Serial Number: *008637*
Test Date: *03/19/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Varnell, Bryon L*
Permit Number: *0036-1210*
Effective:
08/14/2019-08/14/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG716201
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	9:14pm
AIR BLK	.00	9:15pm
ACCY CHK	.07	9:16pm
AIR BLK	.00	9:16pm
SUB TEST	**.00**	**9:17pm**
AIR BLK	.00	9:18pm
SUB TEST	**.00**	**9:19pm**
AIR BLK	.00	9:20pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAYNE COUNTY BAT MOBILE UNIT 6 950

Serial Number: *008637* Test Record Number: *3061*
Test Date: *03/19/2020* Test Time: *9:22pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:22pm
FLO	Pass	9:22pm
FC	Pass	9:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:23pm
SRC	Pass	9:23pm
DET	Pass	9:23pm
BAR	Pass	9:23pm
BT	Pass	9:23pm

Blank Tests

Test	Status	Time
AIR	Pass	9:23pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:23pm

CRC Tests

Test	Status	Time
COMP	Pass	9:24pm
CAL	Pass	9:24pm

Preventive Maintenance
Status: Pass

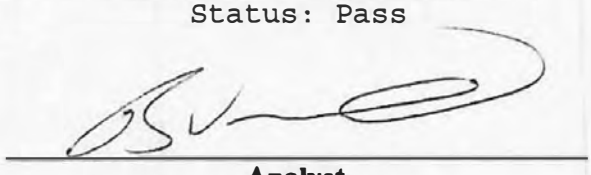

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Wayne Instrument Location Seymour Johnson A.F.B.

Instrument Serial No. 008786 1010 Vermont Garrison Rd., Goldsboro N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd **day of** MARCH, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAYNE COUNTY SEYMOUR JOHNSON AFB 950

Serial Number: *008786*
Test Date: *03/23/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Linda A*
Permit Number: *11646E*
Effective:
07/08/2019-07/08/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG814901
Exp Date: 05/29/2020

Test	g/210L	Time
DIAG	Pass	2:33pm
AIR BLK	.00	2:34pm
ACCY CHK	.08	2:34pm
AIR BLK	.00	2:35pm
SUB TEST	**.00**	**2:36pm**
AIR BLK	.00	2:37pm
SUB TEST	**.00**	**2:38pm**
AIR BLK	.00	2:39pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAYNE COUNTY SEYMOUR JOHNSON AFB 950

Serial Number: *008786* Test Record Number: *343*
Test Date: *03/23/2020* Test Time: *2:41pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:41pm
FLO	Pass	2:41pm
FC	Pass	2:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:41pm
SRC	Pass	2:41pm
DET	Pass	2:41pm
BAR	Pass	2:41pm
BT	Pass	2:41pm

Blank Tests

Test	Status	Time
AIR	Pass	2:42pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:42pm

CRC Tests

Test	Status	Time
COMP	Pass	2:42pm
CAL	Pass	2:42pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Wilson Instrument Location Wilson Co. Detention CTR.

Instrument Serial No. 008627 100 E. Green St, Wilson, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th **day of** MARCH **, 20**20**, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

447
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILSON COUNTY DETENTION CENTER 970

Serial Number: *008627*
Test Date: *03/18/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Linda A*
Permit Number: *0045-5468*
Effective:
07/08/2019-07/08/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG911506
Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	12:39pm
AIR BLK	.00	12:39pm
ACCY CHK	.08	12:40pm
AIR BLK	.00	12:41pm
SUB TEST	**.00**	**12:42pm**
AIR BLK	.00	12:43pm
SUB TEST	**.00**	**12:44pm**
AIR BLK	.00	12:45pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Linda A. Keesler
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WILSON COUNTY DETENTION CENTER 970

Serial Number: *008627* Test Record Number: *2505*
Test Date: *03/18/2020* Test Time: *12:46pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:46pm
FLO	Pass	12:46pm
FC	Pass	12:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:46pm
SRC	Pass	12:46pm
DET	Pass	12:46pm
BAR	Pass	12:46pm
BT	Pass	12:46pm

Blank Tests

Test	Status	Time
AIR	Pass	12:47pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:47pm

CRC Tests

Test	Status	Time
COMP	Pass	12:47pm
CAL	Pass	12:47pm

Preventive Maintenance
Status: Pass

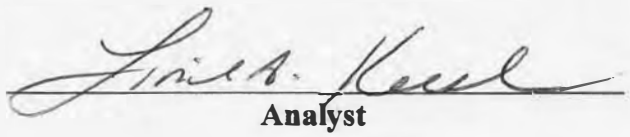

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Wilson Instrument Location Wilson Co. Detention CTR.

Instrument Serial No. 008657 100 E. Green St, Wilson, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th **day of** MARCH, 2020, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILSON COUNTY DETENTION CENTER 970

Serial Number: *008652*
Test Date: *03/18/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Keesler, Linda A*
Permit Number: *0045-5468*
Effective:
07/08/2019-07/08/2021

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG919901
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	12:40pm
AIR BLK	.00	12:41pm
ACCY CHK	.08	12:42pm
AIR BLK	.00	12:43pm
SUB TEST	**.00**	**12:43pm**
AIR BLK	.00	12:44pm
SUB TEST	**.00**	**12:46pm**
AIR BLK	.00	12:46pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WILSON COUNTY DETENTION CENTER 970

Serial Number: *008652* Test Record Number: *3415*
Test Date: *03/18/2020* Test Time: *12:47pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:48pm
FLO	Pass	12:48pm
FC	Pass	12:48pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:48pm
SRC	Pass	12:48pm
DET	Pass	12:48pm
BAR	Pass	12:48pm
BT	Pass	12:48pm

Blank Tests

Test	Status	Time
AIR	Pass	12:49pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:49pm

CRC Tests

Test	Status	Time
COMP	Pass	12:49pm
CAL	Pass	12:49pm

Preventive Maintenance
Status: Pass

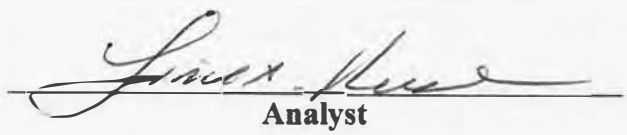

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Yadkin Instrument Location Yadkin Co. Jail

Instrument Serial No. 005854 Yadkinville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 **day of** March, 20 20, **the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

YADKIN COUNTY YADKIN CO JAIL 980

Serial Number: *008854*
Test Date: *03/17/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BURNETTE, ANTHONY J*
Permit Number: *11304E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG821801
Exp Date: 08/06/2020

Test	g/210L	Time
DIAG	Pass	3:16pm
AIR BLK	.00	3:17pm
ACCY CHK	.08	3:18pm
AIR BLK	.00	3:19pm
SUB TEST	**.00**	**3:20pm**
AIR BLK	.00	3:20pm
SUB TEST	**.00**	**3:22pm**
AIR BLK	.00	3:23pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

YADKIN COUNTY YADKIN CO JAIL 980

Serial Number: *008854* Test Record Number: *676*
Test Date: *03/17/2020* Test Time: *3:24pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:24pm
FLO	Pass	3:24pm
FC	Pass	3:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:25pm
SRC	Pass	3:25pm
DET	Pass	3:25pm
BAR	Pass	3:25pm
BT	Pass	3:25pm

Blank Tests

Test	Status	Time
AIR	Pass	3:25pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:25pm

CRC Tests

Test	Status	Time
COMP	Pass	3:25pm
CAL	Pass	3:25pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Yadkin Instrument Location Yadkin Co. Jail

Instrument Serial No. 008944 Yadkinville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 **day of** March **, 20** 20**, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.**

Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (11/07)

Intox EC/IR-II: Subject Test

YADKIN COUNTY YADKIN CO JAIL 980

Serial Number: *008944*
Test Date: *03/17/2020*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BURNETTE, ANTHONY J*
Permit Number: *11304E*
Effective:
06/01/2019-06/01/2021

Officer's Name: *NONE,*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG821401
Exp Date: 08/02/2020

Test	g/210L	Time
DIAG	Pass	3:17pm
AIR BLK	.00	3:18pm
ACCY CHK	.08	3:19pm
AIR BLK	.00	3:19pm
SUB TEST	**.00**	**3:20pm**
AIR BLK	.00	3:21pm
SUB TEST	**.00**	**3:23pm**
AIR BLK	.00	3:23pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

YADKIN COUNTY YADKIN CO JAIL 980

Serial Number: *008944* Test Record Number: *1605*
Test Date: *03/17/2020* Test Time: *3:24pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:25pm
FLO	Pass	3:25pm
FC	Pass	3:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:25pm
SRC	Pass	3:25pm
DET	Pass	3:25pm
BAR	Pass	3:25pm
BT	Pass	3:25pm

Blank Tests

Test	Status	Time
AIR	Pass	3:25pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:26pm

CRC Tests

Test	Status	Time
COMP	Pass	3:26pm
CAL	Pass	3:26pm

Preventive Maintenance
Status: Pass

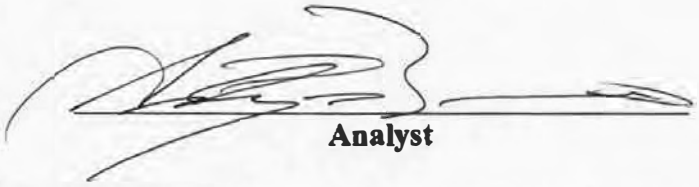

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007