

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Avery Instrument Location Banner EIK PD
Instrument Serial No. 008724 Banner EIK, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

AVERY COUNTY BANNER ELK PD 050

Serial Number: 008724
Test Date: 08/09/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J
Permit Number: 11304E
Effective:
06/01/2019-06/01/2021

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG902201
Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	6:14pm
AIR BLK	.00	6:15pm
ACCY CHK	.07	6:16pm
AIR BLK	.00	6:16pm
SUB TEST	.00	6:17pm
AIR BLK	.00	6:18pm
SUB TEST	.00	6:20pm
AIR BLK	.00	6:20pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

AVERY COUNTY BANNER ELK PD 050

Serial Number: 008724 Test Record Number: 625
Test Date: 08/09/2020 Test Time: 6:22pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:23pm
FLO	Pass	6:23pm
FC	Pass	6:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:23pm
SRC	Pass	6:23pm
DET	Pass	6:23pm
BAR	Pass	6:23pm
BT	Pass	6:23pm

Blank Tests

Test	Status	Time
AIR	Pass	6:23pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:23pm

CRC Tests

Test	Status	Time
COMP	Pass	6:24pm
CAL	Pass	6:24pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Beaufort Instrument Location Belhaven P.D.

Instrument Serial No. 008928 125 W. Main St, Belhaven, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Kou
Signature of Certifying Official

6043
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BEAUFORT COUNTY BELHAVEN PD 060

Serial Number: 008928

Test Date: 08/18/2020

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GUARD, KELLY G

Permit Number: 12955E

Effective:

06/01/2019-06/01/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG902201

Exp Date: 01/22/2021


Test	g/210L	Time
DIAG	Pass	11:12am
AIR BLK	.00	11:13am
ACCY CHK	.08	11:13am
AIR BLK	.00	11:14am
SUB TEST	.00	11:15am
AIR BLK	.00	11:16am
SUB TEST	.00	11:17am
AIR BLK	.00	11:18am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

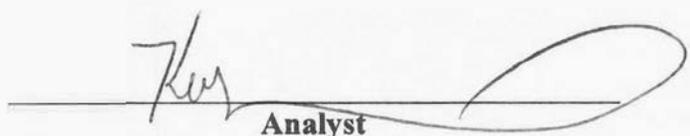

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BEAUFORT COUNTY BELHAVEN PD 060

Serial Number: 008928 Test Record Number: 428
Test Date: 08/18/2020 Test Time: 11:19am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:19am
FLO	Pass	11:19am
FC	Pass	11:19am

Temperature Tests

Test	Status	Time
FC1	Pass	11:20am
SRC	Pass	11:20am
DET	Pass	11:20am
BAR	Pass	11:20am
BT	Pass	11:20am

Blank Tests

Test	Status	Time
AIR	Pass	11:20am

Printer Tests

Test	Status	Time
PRNT	Pass	11:20am

CRC Tests

Test	Status	Time
COMP	Pass	11:20am
CAL	Pass	11:20am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Caswell Instrument Location Caswell Co Detention Ctr

Instrument Serial No. 008593 211 County Park Rd Yanceyville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CASWELL COUNTY DETENTION CENTER 160

Serial Number: 008593
Test Date: 08/03/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, STOKES
Permit Number: 11434E
Effective:
04/01/2019-04/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG919902
Exp Date: 07/18/2021


Test	g/210L	Time
DIAG	Pass	10:46am
AIR BLK	.00	10:46am
ACCY CHK	.08	10:47am
AIR BLK	.00	10:48am
SUB TEST	.00	10:48am
AIR BLK	.00	10:49am
SUB TEST	.00	10:51am
AIR BLK	.00	10:52am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CASWELL COUNTY DETENTION CENTER 160

Serial Number: 008593 Test Record Number: 1817
Test Date: 08/03/2020 Test Time: 10:52am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:53am
FLO	Pass	10:53am
FC	Pass	10:53am

Temperature Tests

Test	Status	Time
FC1	Pass	10:53am
SRC	Pass	10:53am
DET	Pass	10:53am
BAR	Pass	10:53am
BT	Pass	10:53am

Blank Tests

Test	Status	Time
AIR	Pass	10:53am

Printer Tests

Test	Status	Time
PRNT	Pass	10:53am

CRC Tests

Test	Status	Time
COMP	Pass	10:54am
CAL	Pass	10:54am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Catawba Instrument Location Hickory PD

Instrument Serial No. 008841

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

656
Certificate Number

Intox EC/IR-II: Subject Test

CATAWBA COUNTY HICKORY PD 170

Serial Number: 008841
Test Date: 08/05/2020

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hays, Mark D

Permit Number: 0011-3099

Effective:

11/13/2019-11/13/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018401

Exp Date: 07/02/2022


Test	g/210L	Time
DIAG	Pass	2:49pm
AIR BLK	.00	2:50pm
ACCY CHK	.08	2:50pm
AIR BLK	.00	2:51pm
SUB TEST	.00	2:52pm
AIR BLK	.00	2:53pm
SUB TEST	.00	2:54pm
AIR BLK	.00	2:55pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY HICKORY PD 170

Serial Number: 008841 Test Record Number: 2060
Test Date: 08/05/2020 Test Time: 2:57pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:57pm
FLO	Pass	2:57pm
FC	Pass	2:57pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:57pm
SRC	Pass	2:57pm
DET	Pass	2:57pm
BAR	Pass	2:57pm
BT	Pass	2:57pm

Blank Tests

Test	Status	Time
AIR	Pass	2:58pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:58pm

CRC Tests

Test	Status	Time
COMP	Pass	2:58pm
CAL	Pass	2:58pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Catawba Instrument Location Catawba County SO
Instrument Serial No. 008927 100 B Southwest Blvd, Newton

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14th day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hulet
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008927
Test Date: 08/14/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Hutchinson, Joseph E
Permit Number: 0035-6075
Effective:
07/09/2019-07/09/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG933901
Exp Date: 12/05/2021


Test	g/210L	Time
DIAG	Pass	4:04pm
AIR BLK	.00	4:05pm
ACCY CHK	.08	4:06pm
AIR BLK	.00	4:07pm
SUB TEST	.00	4:07pm
AIR BLK	.00	4:08pm
SUB TEST	.00	4:10pm
AIR BLK	.00	4:10pm

Reported AC: .00 g/210L

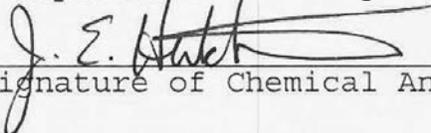

Signature of Chemical Analyst

Court CVR

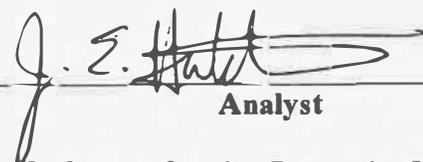

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008927 Test Record Number: 579
Test Date: 08/14/2020 Test Time: 4:11pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:11pm
FLO	Pass	4:11pm
FC	Pass	4:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:12pm
SRC	Pass	4:12pm
DET	Pass	4:12pm
BAR	Pass	4:12pm
BT	Pass	4:12pm

Blank Tests

Test	Status	Time
IR	Pass	4:12pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:12pm

CRC Tests

Test	Status	Time
COMP	Pass	4:13pm
CAL	Pass	4:13pm

Preventive Maintenance
Status: Pass

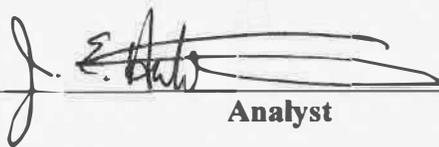

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County CHATHAM Instrument Location CHATHAM Co. Detention Center
Instrument Serial No. 008591 PITTSBORO, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5TH day of AUGUST, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHATHAM COUNTY DETENTION CENTER 180

Serial Number: 008591
Test Date: 08/05/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: *Galloway, Charles L*
Permit Number: 0023-9771
Effective:
02/17/2020-02/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG934001
Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	1:57pm
AIR BLK	.00	1:58pm
ACCY CHK	.08	1:58pm
AIR BLK	.00	1:59pm
SUB TEST	.00	2:00pm
AIR BLK	.00	2:01pm
SUB TEST	.00	2:02pm
AIR BLK	.00	2:03pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CHATHAM COUNTY DETENTION CENTER 180

Serial Number: 008591 Test Record Number: 2381
Test Date: 08/05/2020 Test Time: 2:05pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:05pm
FLO	Pass	2:05pm
FC	Pass	2:05pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:05pm
SRC	Pass	2:05pm
DET	Pass	2:05pm
BAR	Pass	2:05pm
BT	Pass	2:05pm

Blank Tests

Test	Status	Time
AIR	Pass	2:06pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:06pm

CRC Tests

Test	Status	Time
COMP	Pass	2:06pm
CAL	Pass	2:06pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Chowan Instrument Location Chowan Public Safety Center

Instrument Serial No. 008855 305 FREEMASON ST, EDENTON,
N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of AUGUST, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Lisa M. Keel
Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHOWAN COUNTY PUBLIC SAFETY CENTER 200

Serial Number: 008895
Test Date: 08/05/2020

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Keesler, Linda A

Permit Number: 0045-5468

Effective:

07/08/2019-07/08/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG902201

Exp Date: 01/22/2021


Test	g/210L	Time
DIAG	Pass	11:57am
AIR BLK	.00	11:58am
ACCY CHK	.07	11:59am
AIR BLK	.00	12:00pm
SUB TEST	.00	12:01pm
AIR BLK	.00	12:01pm
SUB TEST	.00	12:03pm
AIR BLK	.00	12:04pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CHOWAN COUNTY PUBLIC SAFETY CENTER 200

Serial Number: 008895 Test Record Number: 976
Test Date: 08/05/2020 Test Time: 12:05pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:05pm
FLO	Pass	12:05pm
FC	Pass	12:05pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:05pm
SRC	Pass	12:05pm
DET	Pass	12:05pm
BAR	Pass	12:05pm
BT	Pass	12:05pm

Blank Tests

Test	Status	Time
AIR	Pass	12:06pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:06pm

CRC Tests

Test	Status	Time
COMP	Pass	12:06pm
CAL	Pass	12:06pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County CURRITUCK Instrument Location CURRITUCK CO.S.D - COROLLA
Instrument Serial No. 008949 1123 Ocean trail, Corolla, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Linda Kuse
Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CURRITUCK COUNTY SO-COROLLA 260

Serial Number: 008949

Test Date: 08/26/2020

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Keesler, Linda A

Permit Number: 0045-5468

Effective:

07/08/2019-07/08/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601


Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	1:53pm
AIR BLK	.00	1:54pm
ACCY CHK	.08	1:54pm
AIR BLK	.00	1:55pm
SUB TEST	.00	1:57pm
AIR BLK	.00	1:57pm
SUB TEST	.00	1:59pm
AIR BLK	.00	2:00pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CURRITUCK COUNTY SO-COROLLA 260

Serial Number: 008949 Test Record Number: 558
Test Date: 08/26/2020 Test Time: 2:01pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:01pm
FLO	Pass	2:01pm
FC	Pass	2:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:02pm
SRC	Pass	2:02pm
DET	Pass	2:02pm
BAR	Pass	2:02pm
BT	Pass	2:02pm

Blank Tests

Test	Status	Time
AIR	Pass	2:02pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:02pm

CRC Tests

Test	Status	Time
COMP	Pass	2:02pm
CAL	Pass	2:02pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County DARE Instrument Location Kill Devil Hills P.D.
Instrument Serial No. 008844 102 Town Dr., Kill Devil Hills, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of AUGUST, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Linda A. Rush
Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY KILL DEVIL HILLS PD 270

Serial Number: 008844
Test Date: 08/26/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Keesler, Linda A
Permit Number: 0045-5468
Effective:
07/08/2019-07/08/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022


Test	g/210L	Time
DIAG	Pass	12:27pm
AIR BLK	.00	12:28pm
ACCY CHK	.08	12:29pm
AIR BLK	.00	12:30pm
SUB TEST	.00	12:30pm
AIR BLK	.00	12:31pm
SUB TEST	.00	12:33pm
AIR BLK	.00	12:34pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY KILL DEVIL HILLS PD 270

Serial Number: 008844 Test Record Number: 2405
Test Date: 08/26/2020 Test Time: 12:35pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:36pm
FLO	Pass	12:36pm
FC	Pass	12:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:36pm
SRC	Pass	12:36pm
DET	Pass	12:36pm
BAR	Pass	12:36pm
BT	Pass	12:36pm

Blank Tests

Test	Status	Time
AIR	Pass	12:36pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:37pm

CRC Tests

Test	Status	Time
COMP	Pass	12:37pm
CAL	Pass	12:37pm

Preventive Maintenance
Status: Pass

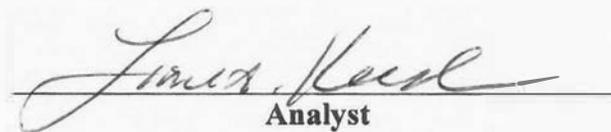
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County DAVIDSON Instrument Location THOMASVILLE

Instrument Serial No. 008872 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18TH day of AUGUST, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY THOMASVILLE PD 280

Serial Number: 008872

Test Date: 08/18/2020

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG919901

Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	12:38pm
AIR BLK	.00	12:39pm
ACCY CHK	.07	12:40pm
AIR BLK	.00	12:41pm
SUB TEST	.00	12:41pm
AIR BLK	.00	12:42pm
SUB TEST	.00	12:43pm
AIR BLK	.00	12:44pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY THOMASVILLE PD 280

Serial Number: 008872 Test Record Number: 1488
Test Date: 08/18/2020 Test Time: 12:45pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:46pm
FLO	Pass	12:46pm
FC	Pass	12:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:46pm
SRC	Pass	12:46pm
DET	Pass	12:46pm
BAR	Pass	12:46pm
BT	Pass	12:46pm

Blank Tests

Test	Status	Time
AIR	Pass	12:47pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:47pm

CRC Tests

Test	Status	Time
COMP	Pass	12:47pm
CAL	Pass	12:47pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Durham Instrument Location Durham Co Jail

Instrument Serial No. 00 8859 219 S. Mangum St. Durham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008859
Test Date: 08/03/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, STOKES
Permit Number: 11434E
Effective:
04/01/2019-04/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG933703
Exp Date: 12/03/2021


Test	g/210L	Time
DIAG	Pass	1:57pm
AIR BLK	.00	1:57pm
ACCY CHK	.08	1:58pm
AIR BLK	.00	1:59pm
SUB TEST	.00	2:00pm
AIR BLK	.00	2:00pm
SUB TEST	.00	2:02pm
AIR BLK	.00	2:03pm

Reported AC: 00 g/210L



Signature of Chemical Analyst

Court CVR

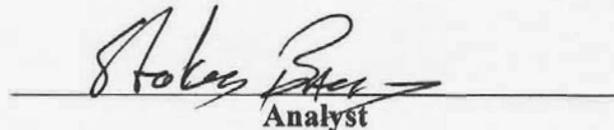

Analyst

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008859 Test Record Number: 2404
Test Date: 08/03/2020 Test Time: 2:04pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:04pm
FLO	Pass	2:04pm
FC	Pass	2:04pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:04pm
SRC	Pass	2:04pm
DET	Pass	2:04pm
BAR	Pass	2:04pm
BT	Pass	2:04pm

Blank Tests

Test	Status	Time
AIR	Pass	2:05pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:05pm

CRC Tests

Test	Status	Time
COMP	Pass	2:05pm
CAL	Pass	2:05pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Durham Instrument Location Durham Co Jail

Instrument Serial No. 00 8878 219 S. Mangum St Durham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008878
Test Date: 08/03/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, STOKES
Permit Number: 11434E
Effective:
04/01/2019-04/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG933703
Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	1:53pm
AIR BLK	.00	1:54pm
ACCY CHK	.08	1:55pm
AIR BLK	.00	1:56pm
SUB TEST	.00	1:57pm
AIR BLK	.00	1:58pm
SUB TEST	.00	1:59pm
AIR BLK	.00	2:00pm

Reported AC: 00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008878 Test Record Number: 4888
Test Date: 08/03/2020 Test Time: 2:01pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:01pm
FLO	Pass	2:01pm
FC	Pass	2:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:01pm
SRC	Pass	2:01pm
DET	Pass	2:01pm
BAR	Pass	2:01pm
BT	Pass	2:01pm

Blank Tests

Test	Status	Time
AIR	Pass	2:02pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:02pm

CRC Tests

Test	Status	Time
COMP	Pass	2:02pm
CAL	Pass	2:02pm

Preventive Maintenance
Status: Pass

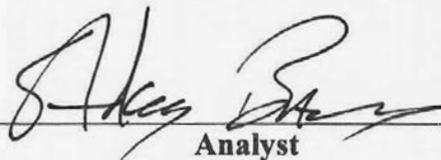
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Durham Instrument Location Durham Co Jail
Instrument Serial No. 008891 219 S. Main St. Durham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008891
Test Date: 08/03/2020

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, STOKES

Permit Number: 11434E

Effective:

04/01/2019-04/01/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG933703

Exp Date: 12/03/2021


Test	g/210L	Time
DIAG	Pass	1:54pm
AIR BLK	.00	1:55pm
ACCY CHK	.08	1:56pm
AIR BLK	.00	1:57pm
SUB TEST	.00	1:58pm
AIR BLK	.00	1:59pm
SUB TEST	.00	2:00pm
AIR BLK	.00	2:01pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

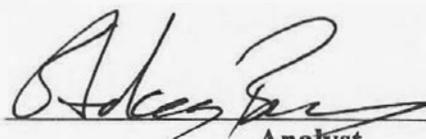

Analyst

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008891 Test Record Number: 4242
Test Date: 08/03/2020 Test Time: 2:02pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:02pm
FLO	Pass	2:02pm
FC	Pass	2:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:02pm
SRC	Pass	2:02pm
DET	Pass	2:02pm
BAR	Pass	2:02pm
BT	Pass	2:02pm

Blank Tests

Test	Status	Time
AIR	Pass	2:03pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:03pm

CRC Tests

Test	Status	Time
COMP	Pass	2:03pm
CAL	Pass	2:03pm

Preventive Maintenance
Status: Pass

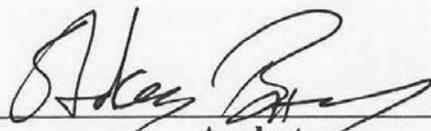

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Forsyth Instrument Location Forsyth Co Detention
Instrument Serial No. 008542 Winston-Salem, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY FORSYTH CO DETENTION
330

Serial Number: 008583
Test Date: 08/03/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J
Permit Number: 11304E
Effective:
06/01/2019-00/00/0000

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG919901
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	3:16pm
AIR BLK	.00	3:17pm
ACCY CHK	.08	3:18pm
AIR BLK	.00	3:19pm
SUB TEST	.00	3:19pm
AIR BLK	.00	3:20pm
SUB TEST	.00	3:22pm
AIR BLK	.00	3:23pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

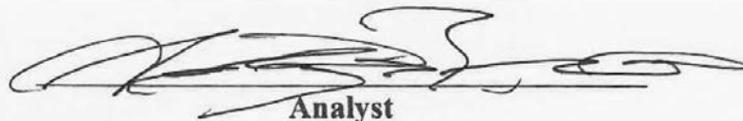

Analyst

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY FORSYTH CO DETENTION 330

Serial Number: 008583 Test Record Number: 8186
Test Date: 08/03/2020 Test Time: 3:26pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:26pm
FLO	Pass	3:26pm
FC	Pass	3:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:27pm
SRC	Pass	3:27pm
DET	Pass	3:27pm
BAR	Pass	3:27pm
BT	Pass	3:27pm

Blank Tests

Test	Status	Time
AIR	Pass	3:27pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:27pm

CRC Tests

Test	Status	Time
COMP	Pass	3:27pm
CAL	Pass	3:27pm

Preventive Maintenance
Status: Pass

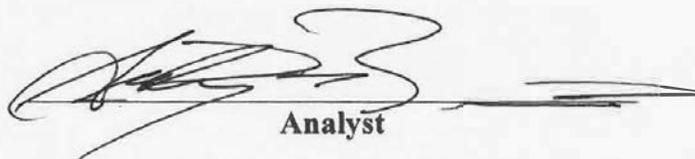
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Forsyth Instrument Location Kernersville

Instrument Serial No. 008650 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY KERNERSVILLE PD 330

Serial Number: 008650
Test Date: 08/12/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J
Permit Number: 11304E
Effective:
06/01/2019-06/01/2021

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG933901
Exp Date: 12/05/2021

Test	g/210L	Time
DIAG	Pass	4:33pm
AIR BLK	.00	4:34pm
ACCY CHK	.08	4:35pm
AIR BLK	.00	4:36pm
SUB TEST	.00	4:36pm
AIR BLK	.00	4:37pm
SUB TEST	.00	4:39pm
AIR BLK	.00	4:39pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY KERNERSVILLE PD 330

Serial Number: 008650 Test Record Number: 1628
Test Date: 08/12/2020 Test Time: 4:41pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:41pm
FLO	Pass	4:41pm
FC	Pass	4:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:41pm
SRC	Pass	4:41pm
DET	Pass	4:41pm
BAR	Pass	4:41pm
BT	Pass	4:41pm

Blank Tests

Test	Status	Time
AIR	Pass	4:42pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:42pm

CRC Tests

Test	Status	Time
COMP	Pass	4:42pm
CAL	Pass	4:42pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Forsyth Instrument Location Forsyth Co. Detention

Instrument Serial No. 208659 Winston-Salem, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY FORSYTH CO DETENTION
330

Serial Number: 008659
Test Date: 08/03/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J
Permit Number: 11304E
Effective:
06/01/2019-06/01/2021

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG919902
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	3:16pm
AIR BLK	.00	3:16pm
ACCY CHK	.08	3:17pm
AIR BLK	.00	3:18pm
SUB TEST	.00	3:19pm
AIR BLK	.00	3:20pm
SUB TEST	.00	3:22pm
AIR BLK	.00	3:22pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

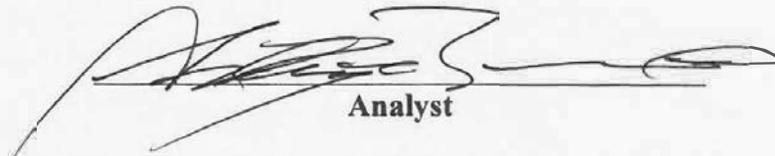

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY FORSYTH CO DETENTION 330

Serial Number: 008659 Test Record Number: 5509
Test Date: 08/03/2020 Test Time: 3:26pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:26pm
FLO	Pass	3:26pm
FC	Pass	3:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:27pm
SRC	Pass	3:27pm
DET	Pass	3:27pm
BAR	Pass	3:27pm
BT	Pass	3:27pm

Blank Tests

Test	Status	Time
AIR	Pass	3:27pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:27pm

CRC Tests

Test	Status	Time
COMP	Pass	3:27pm
CAL	Pass	3:27pm

Preventive Maintenance
Status: Pass

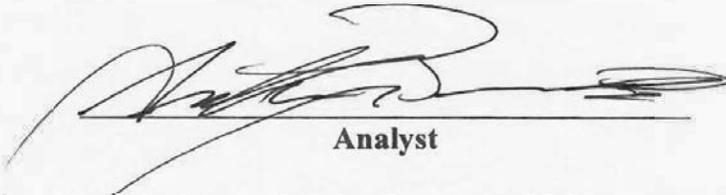

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Forsyth Instrument Location Forsyth Co. Detention

Instrument Serial No. 008925 Winston-Salem

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

1649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY FORSYTH CO DETENTION
330

Serial Number: 008925
Test Date: 08/03/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J
Permit Number: 11304E
Effective:
06/01/2019-06/01/2021

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG933901
Exp Date: 12/05/2021

Test	g/210L	Time
DIAG	Pass	3:17pm
AIR BLK	.00	3:18pm
ACCY CHK	.08	3:19pm
AIR BLK	.00	3:19pm
SUB TEST	.00	3:20pm
AIR BLK	.00	3:21pm
SUB TEST	.00	3:23pm
AIR BLK	.00	3:23pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

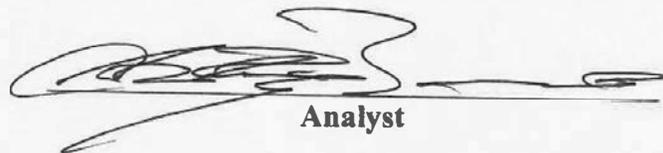

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY FORSYTH CO DETENTION 330

Serial Number: 008925 Test Record Number: 3308
Test Date: 08/03/2020 Test Time: 3:26pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:26pm
FLO	Pass	3:26pm
FC	Pass	3:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:26pm
SRC	Pass	3:26pm
DET	Pass	3:26pm
BAR	Pass	3:26pm
BT	Pass	3:26pm

Blank Tests

Test	Status	Time
AIR	Pass	3:27pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:27pm

CRC Tests

Test	Status	Time
COMP	Pass	3:27pm
CAL	Pass	3:27pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Gates Instrument Location Gates Co. S.O.
Instrument Serial No. 008884 202 Court St., Gatesville, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Kelly

Signature of Certifying Official

643

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GATES COUNTY GATES CO SO 360

Serial Number: 008884
Test Date: 08/05/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: GUARD, KELLY G
Permit Number: 12955E
Effective:
06/01/2019-06/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022


Test	g/210L	Time
DIAG	Pass	10:44am
AIR BLK	.00	10:45am
ACCY CHK	.07	10:46am
AIR BLK	.00	10:47am
SUB TEST	.00	10:47am
AIR BLK	.00	10:48am
SUB TEST	.00	10:50am
AIR BLK	.00	10:51am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

GATES COUNTY GATES CO SO 360

Serial Number: 008884 Test Record Number: 960
Test Date: 08/05/2020 Test Time: 10:51am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:52am
FLO	Pass	10:52am
FC	Pass	10:52am

Temperature Tests

Test	Status	Time
FC1	Pass	10:52am
SRC	Pass	10:52am
DET	Pass	10:52am
BAR	Pass	10:52am
BT	Pass	10:52am

Blank Tests

Test	Status	Time
AIR	Pass	10:53am

Printer Tests

Test	Status	Time
PRNT	Pass	10:53am

CRC Tests

Test	Status	Time
COMP	Pass	10:53am
CAL	Pass	10:53am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Granville Instrument Location Creedmore PD

Instrument Serial No 008641 111 Masonic St. Creedmore, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

462
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GRANVILLE COUNTY CREEDMOOR PD 380

Serial Number: 008641
Test Date: 08/04/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, STOKES
Permit Number: 11434E
Effective:
04/01/2019-04/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG919902
Exp Date: 07/18/2021


Test	g/210L	Time
DIAG	Pass	1:10pm
AIR BLK	.00	1:11pm
ACCY CHK	.08	1:11pm
AIR BLK	.00	1:12pm
SUB TEST	.00	1:13pm
AIR BLK	.00	1:14pm
SUB TEST	.00	1:15pm
AIR BLK	.00	1:16pm

Reported AC: .00 g/210L

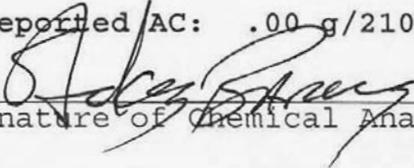

Signature of Chemical Analyst

Court CVR

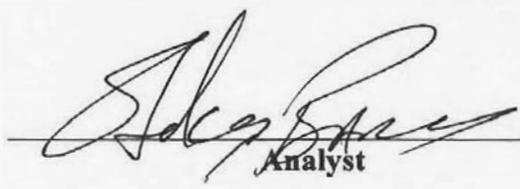

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GRANVILLE COUNTY CREEDMOOR PD 380

Serial Number: 008641 Test Record Number: 1312
Test Date: 08/04/2020 Test Time: 1:16pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:17pm
FLO	Pass	1:17pm
FC	Pass	1:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:17pm
SRC	Pass	1:17pm
DET	Pass	1:17pm
BAR	Pass	1:17pm
BT	Pass	1:17pm

Blank Tests

Test	Status	Time
AIR	Pass	1:18pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:18pm

CRC Tests

Test	Status	Time
COMP	Pass	1:18pm
CAL	Pass	1:18pm

Preventive Maintenance
Status: Pass

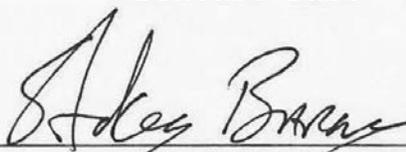

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Granville Instrument Location OXFORD PD

Instrument Serial No. 008923 201 E. McClanahan St. OXFORD NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alex Barnes
Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GRANVILLE COUNTY OXFORD PD 380

Serial Number: 008923
Test Date: 08/04/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, STOKES
Permit Number: 11434E
Effective:
04/01/2019-04/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018401
Exp Date: 07/02/2022


Test	g/210L	Time
DIAG	Pass	10:05am
AIR BLK	.00	10:06am
ACCY CHK	.07	10:06am
AIR BLK	.00	10:07am
SUB TEST	.00	10:08am
AIR BLK	.00	10:09am
SUB TEST	.00	10:10am
AIR BLK	.00	10:11am

Reported AC: 00 g/210L



Signature of Chemical Analyst

Court CVR

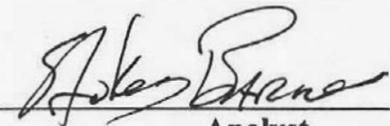

Analyst

Intox EC/IR-II: Preventive Maintenance

GRANVILLE COUNTY OXFORD PD 380

Serial Number: 008923 Test Record Number: 2429
Test Date: 08/04/2020 Test Time: 10:16am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:17am
FLO	Pass	10:17am
FC	Pass	10:17am

Temperature Tests

Test	Status	Time
FC1	Pass	10:17am
SRC	Pass	10:17am
DET	Pass	10:17am
BAR	Pass	10:17am
BT	Pass	10:17am

Blank Tests

Test	Status	Time
AIR	Pass	10:18am

Printer Tests

Test	Status	Time
PRNT	Pass	10:18am

CRC Tests

Test	Status	Time
COMP	Pass	10:18am
CAL	Pass	10:18am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Guilford Instrument Location UNC - Greensboro

Instrument Serial No. 008604 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY UNC-G POLICE DEPT 400

Serial Number: 008604

Test Date: 08/06/2020

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J

Permit Number: 11304E

Effective:

06/01/2019-06/01/2021

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG933703


Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	7:04pm
AIR BLK	.00	7:05pm
ACCY CHK	.08	7:06pm
AIR BLK	.00	7:07pm
SUB TEST	.00	7:08pm
AIR BLK	.00	7:09pm
SUB TEST	.00	7:10pm
AIR BLK	.00	7:11pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

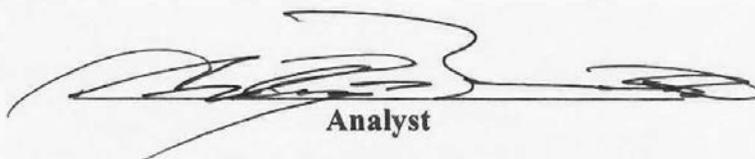

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY UNC-G POLICE DEPT 400

Serial Number: 008604 Test Record Number: 1906
Test Date: 08/06/2020 Test Time: 7:12pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:12pm
FLO	Pass	7:12pm
FC	Pass	7:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:12pm
SRC	Pass	7:12pm
DET	Pass	7:12pm
BAR	Pass	7:12pm
BT	Pass	7:12pm

Blank Tests

Test	Status	Time
AIR	Pass	7:13pm


Printer Tests

Test	Status	Time
PRNT	Pass	7:13pm

CRC Tests

Test	Status	Time
COMP	Pass	7:13pm
CAL	Pass	7:13pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County GUILFORD Instrument Location HIGH POINT JAIL

Instrument Serial No. 008655 HIGH POINT, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18TH day of AUGUST, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY HIGH POINT JAIL 400

Serial Number: 008655
Test Date: 08/18/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Oligmueller Jr., Leo A*
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: *NONE*,
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*


Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	3:16pm
AIR BLK	.00	3:16pm
ACCY CHK	.07	3:17pm
AIR BLK	.00	3:18pm
SUB TEST	.00	3:19pm
AIR BLK	.00	3:20pm
SUB TEST	.00	3:21pm
AIR BLK	.00	3:22pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

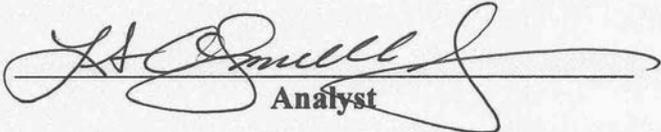
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY HIGH POINT JAIL 400

Serial Number: 008655 Test Record Number: 3578
Test Date: 08/18/2020 Test Time: 3:24pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:24pm
FLO	Pass	3:24pm
FC	Pass	3:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:25pm
SRC	Pass	3:25pm
DET	Pass	3:25pm
BAR	Pass	3:25pm
BT	Pass	3:25pm

Blank Tests

Test	Status	Time
AIR	Pass	3:25pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:25pm

CRC Tests

Test	Status	Time
COMP	Pass	3:25pm
CAL	Pass	3:25pm

Preventive Maintenance
Status: Pass

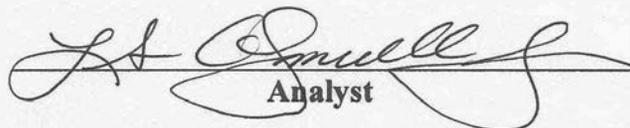
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Guilford Instrument Location Greensboro

Instrument Serial No. 009225 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 649 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GREENSBORO PD 400

Serial Number: 008725
Test Date: 08/10/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J
Permit Number: 11304E
Effective:
06/01/2019-06/01/2021

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG920301
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	3:29pm
AIR BLK	.00	3:30pm
ACCY CHK	.08	3:30pm
AIR BLK	.00	3:31pm
SUB TEST	.00	3:32pm
AIR BLK	.00	3:33pm
SUB TEST	.00	3:34pm
AIR BLK	.00	3:35pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GREENSBORO PD 400

Serial Number: 008725 Test Record Number: 4573
Test Date: 08/10/2020 Test Time: 3:36pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:37pm
FLO	Pass	3:37pm
FC	Pass	3:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:37pm
SRC	Pass	3:37pm
DET	Pass	3:37pm
BAR	Pass	3:37pm
BT	Pass	3:37pm

Blank Tests

Test	Status	Time
AIR	Pass	3:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:37pm

CRC Tests

Test	Status	Time
COMP	Pass	3:38pm
CAL	Pass	3:38pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County HALIFAX Instrument Location Roanoke Rapids PD
Instrument Serial No. 008635 1040 Roanoke Ave
Roanoke Rapids, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HALIFAX CO ROANOKE RAPIDS PD 410

Serial Number: 008635
Test Date: 08/05/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, STOKES
Permit Number: 11434E
Effective:
04/01/2019-04/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG911501
Exp Date: 04/25/2021


Test	g/210L	Time
DIAG	Pass	2:28pm
AIR BLK	.00	2:29pm
ACCY CHK	.08	2:30pm
AIR BLK	.00	2:31pm
SUB TEST	.00	2:31pm
AIR BLK	.00	2:32pm
SUB TEST	.00	2:34pm
AIR BLK	.00	2:35pm

Reported AC: 00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HALIFAX CO ROANOKE RAPIDS PD 410

Serial Number: 008635 Test Record Number: 1795
Test Date: 08/05/2020 Test Time: 2:36pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:37pm
FLO	Pass	2:37pm
FC	Pass	2:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:37pm
SRC	Pass	2:37pm
DET	Pass	2:37pm
BAR	Pass	2:37pm
BT	Pass	2:37pm

Blank Tests

Test	Status	Time
AIR	Pass	2:38pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:38pm

CRC Tests

Test	Status	Time
COMP	Pass	2:38pm
CAL	Pass	2:38pm

Preventive Maintenance
Status: Pass

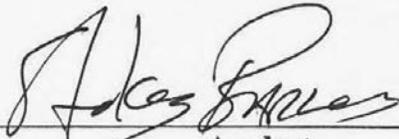

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County HALIFAX Instrument Location Roanoke Rapids PD
Instrument Serial No. 008656 1040 Roanoke Ave
Roanoke Rapids, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Ades Barnes
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HALIFAX CO. ROANOKE RAPIDS PD 410

Serial Number: 008656
Test Date: 08/05/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, STOKES
Permit Number: 11434E
Effective:
04/01/2019-04/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG902201
Exp Date: 01/22/2021


Test	g/210L	Time
DIAG	Pass	2:27pm
AIR BLK	.00	2:28pm
ACCY CHK	.07	2:29pm
AIR BLK	.00	2:30pm
SUB TEST	.00	2:30pm
AIR BLK	.00	2:31pm
SUB TEST	.00	2:32pm
AIR BLK	.00	2:33pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

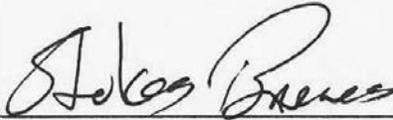

Analyst

Intox EC/IR-II: Preventive Maintenance

HALIFAX CO. ROANOKE RAPIDS PD 410

Serial Number: 008656 Test Record Number: 689
Test Date: 08/05/2020 Test Time: 2:34pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:34pm
FLO	Pass	2:34pm
FC	Pass	2:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:35pm
SRC	Pass	2:35pm
DET	Pass	2:35pm
BAR	Pass	2:35pm
BT	Pass	2:35pm

Blank Tests

Test	Status	Time
AIR	Pass	2:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:35pm

CRC Tests

Test	Status	Time
COMP	Pass	2:35pm
CAL	Pass	2:35pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County HALIFAX Instrument Location HALIFAX CO. S.O.
Instrument Serial No 008695 335 Ferrall Lane Halifax, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of AUGUST, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HALIFAX CO. HALIFAX CO SO 410

Serial Number: 008695
Test Date: 08/05/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, STOKES
Permit Number: 11434E
Effective:
04/01/2019-04/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG911501
Exp Date: 04/25/2021


Test	g/210L	Time
DIAG	Pass	11:31am
AIR BLK	.00	11:32am
ACCY CHK	.08	11:32am
AIR BLK	.00	11:33am
SUB TEST	.00	11:34am
AIR BLK	.00	11:35am
SUB TEST	.00	11:36am
AIR BLK	.00	11:37am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

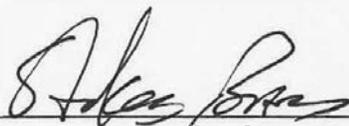

Analyst

Intox EC/IR-II: Preventive Maintenance

HALIFAX CO. HALIFAX CO SO 410

Serial Number: 008695 Test Record Number: 2963
Test Date: 08/05/2020 Test Time: 11:41am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:41am
FLO	Pass	11:41am
FC	Pass	11:41am

Temperature Tests

Test	Status	Time
FC1	Pass	11:41am
SRC	Pass	11:41am
DET	Pass	11:41am
BAR	Pass	11:41am
BT	Pass	11:41am

Blank Tests

Test	Status	Time
AIR	Pass	11:42am


Printer Tests

Test	Status	Time
PRNT	Pass	11:42am

CRC Tests

Test	Status	Time
COMP	Pass	11:42am
CAL	Pass	11:42am

Preventive Maintenance
Status: Pass

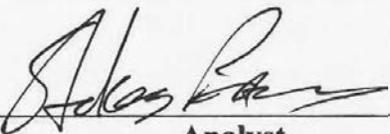

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Henderson Instrument Location Henderson Co Jail
Instrument Serial No. 008822 Hendersonville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of August, 2020 the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HENDERSON COUNTY DETENTION 440

Serial Number: 008822

Test Date: 08/10/2020

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: LOFTIS, BENJAMIN C

Permit Number: 24801E

Effective:

07/01/2019-07/01/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601


Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	12:13pm
AIR BLK	.00	12:14pm
ACCY CHK	.08	12:14pm
AIR BLK	.00	12:15pm
SUB TEST	.00	12:15pm
AIR BLK	.00	12:16pm
SUB TEST	.00	12:18pm
AIR BLK	.00	12:19pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

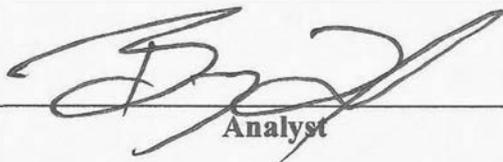
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HENDERSON COUNTY DETENTION 440

Serial Number: 008822 Test Record Number: 2632
Test Date: 08/10/2020 Test Time: 12:21pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:22pm
FLO	Pass	12:22pm
FC	Pass	12:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:22pm
SRC	Pass	12:22pm
DET	Pass	12:22pm
BAR	Pass	12:22pm
BT	Pass	12:22pm

Blank Tests

Test	Status	Time
AIR	Pass	12:22pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:23pm

CRC Tests

Test	Status	Time
COMP	Pass	12:23pm
CAL	Pass	12:23pm

Preventive Maintenance
Status: Pass

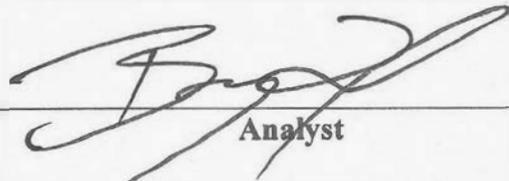
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Iredell Instrument Location CARMOBILE #3
Instrument Serial No. 008002 NCWRC
LAKE NORMAN

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

659
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL BAT MOBILE 3 480

Serial Number: 008002
Test Date: 08/08/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 01/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ingle, Larry W
Permit Number: 0035-2495
Effective:
01/09/2020-01/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022


Test	g/210L	Time
DIAG	Pass	5:53pm
AIR BLK	.00	5:54pm
ACCY CHK	.08	5:54pm
AIR BLK	.00	5:55pm
SUB TEST	.00	5:56pm
AIR BLK	.00	5:57pm
SUB TEST	.00	5:58pm
AIR BLK	.00	5:59pm

Reported AC: .00 g/210L

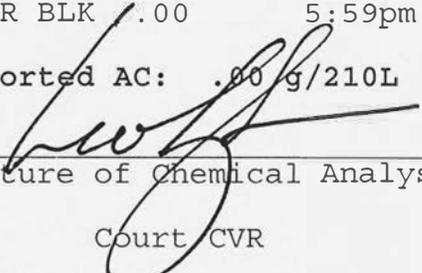

Signature of Chemical Analyst

Court CVR

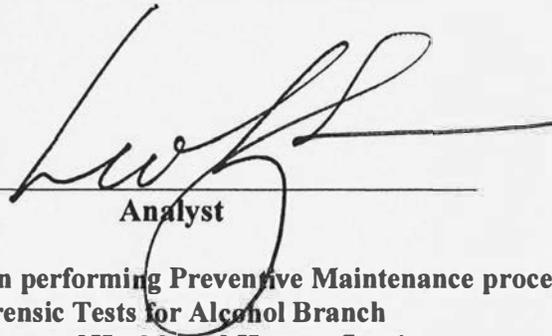

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

IREDELL BAT MOBILE 3 480

Serial Number: 008002 Test Record Number: 557
Test Date: 08/08/2020 Test Time: 6:00pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:01pm
FLO	Pass	6:01pm
FC	Pass	6:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:01pm
SRC	Pass	6:01pm
DET	Pass	6:01pm
BAR	Pass	6:01pm
BT	Pass	6:01pm

Blank Tests

Test	Status	Time
AIR	Pass	6:02pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:02pm

CRC Tests

Test	Status	Time
COMP	Pass	6:02pm
CAL	Pass	6:02pm

Preventive Maintenance
Status: Pass

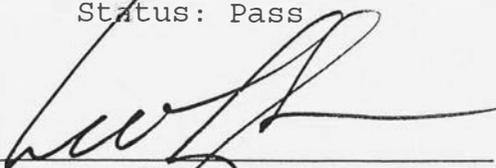

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location Statesville PD

Instrument Serial No. 008619

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Mark J. Hays Signature of Certifying Official 656 Certificate Number

Intox EC/IR-II: Subject Test

IREDELL COUNTY STATESVILLE PD 480

Serial Number: 008619
Test Date: 08/13/2020

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hays, Mark D

Permit Number: 0011-3099

Effective:

11/13/2019-11/13/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	1:42pm
AIR BLK	.00	1:43pm
ACCY CHK	.08	1:43pm
AIR BLK	.00	1:44pm
SUB TEST	.00	1:46pm
AIR BLK	.00	1:47pm
SUB TEST	.00	1:48pm
AIR BLK	.00	1:49pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY STATESVILLE PD 480

Serial Number: 008619 Test Record Number: 1738
Test Date: 08/13/2020 Test Time: 1:50pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:51pm
FLO	Pass	1:51pm
FC	Pass	1:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:51pm
SRC	Pass	1:51pm
DET	Pass	1:51pm
BAR	Pass	1:51pm
BT	Pass	1:51pm

Blank Tests

Test	Status	Time
AIR	Pass	1:51pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:51pm

CRC Tests

Test	Status	Time
COMP	Pass	1:52pm
CAL	Pass	1:52pm

Preventive Maintenance
Status: *Pass*

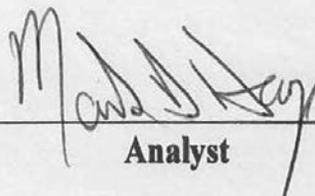

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location Mooreville PD

Instrument Serial No. 008685

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



M. D. [Signature]
Signature of Certifying Official

656
Certificate Number

Intox EC/IR-II: Subject Test

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008685
Test Date: 08/13/2020

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hays, Mark D

Permit Number: 0011-3099

Effective:

11/13/2019-11/13/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018401

Exp Date: 07/02/2022

Test	g/210L	Time
DIAG	Pass	12:18pm
AIR BLK	.00	12:19pm
ACCY CHK	.07	12:20pm
AIR BLK	.00	12:21pm
SUB TEST	.00	12:22pm
AIR BLK	.00	12:23pm
SUB TEST	.00	12:24pm
AIR BLK	.00	12:25pm

Reported AC: .00 g/210L

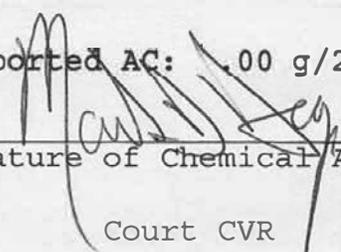

Signature of Chemical Analyst

Court CVR

Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008685 Test Record Number: 3420
Test Date: 08/13/2020 Test Time: 12:26pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:27pm
FLO	Pass	12:27pm
FC	Pass	12:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:27pm
SRC	Pass	12:27pm
DET	Pass	12:27pm
BAR	Pass	12:27pm
BT	Pass	12:27pm

Blank Tests

Test	Status	Time
AIR	Pass	12:27pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:28pm

CRC Tests

Test	Status	Time
COMP	Pass	12:28pm
CAL	Pass	12:28pm

Preventive Maintenance
Status: Pass

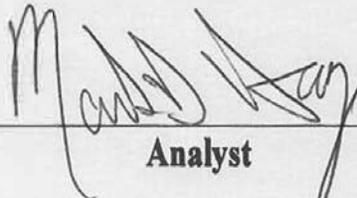

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Iredell Instrument Location Iredell County SO
Instrument Serial No. 008809

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



M. D. [Signature]
Signature of Certifying Official

656
Certificate Number

Intox EC/IR-II: Subject Test

IREDELL COUNTY IREDELL COUNTY SO 480

Serial Number: 008809
Test Date: 08/27/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: *Hays, Mark D*
Permit Number: 0011-3099
Effective:
11/13/2019-11/13/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG919901
Exp Date: 07/18/2021


Test	g/210L	Time
DIAG	Pass	9:14am
AIR BLK	.00	9:15am
ACCY CHK	.08	9:16am
AIR BLK	.00	9:17am
SUB TEST	.00	9:18am
AIR BLK	.00	9:19am
SUB TEST	.00	9:21am
AIR BLK	.00	9:22am

Reported AC: .00 g/210L

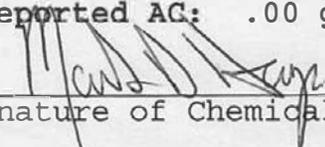

Signature of Chemical Analyst

Court CVR

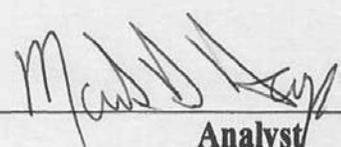

Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY IREDELL COUNTY SO 480

Serial Number: 008809 Test Record Number: 4464
Test Date: 08/27/2020 Test Time: 9:24am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:24am
FLO	Pass	9:24am
FC	Pass	9:24am

Temperature Tests

Test	Status	Time
FC1	Pass	9:24am
SRC	Pass	9:24am
DET	Pass	9:24am
BAR	Pass	9:24am
BT	Pass	9:24am

Blank Tests

Test	Status	Time
AIR	Pass	9:25am


Printer Tests

Test	Status	Time
PRNT	Pass	9:25am

CRC Tests

Test	Status	Time
COMP	Pass	9:25am
CAL	Pass	9:25am

Preventive Maintenance
Status: Pass

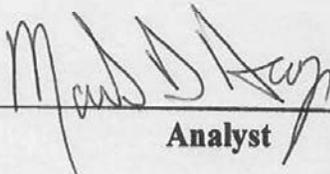

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Tredell Instrument Location Bad Mobile Unit 2

Instrument Serial No. 008970 Wildlife

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrades;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Chris Joy

Signature of Certifying Official

658

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 02 480

Serial Number: 008970
Test Date: 08/22/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: TOWERY, CHAD V
Permit Number: 26632E
Effective:
05/01/2019-05/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG902201
Exp Date: 01/22/2021


Test	g/210L	Time
DIAG	Pass	4:15pm
AIR BLK	.00	4:16pm
ACCY CHK	.08	4:16pm
AIR BLK	.00	4:17pm
SUB TEST	.00	4:18pm
AIR BLK	.00	4:19pm
SUB TEST	.00	4:20pm
AIR BLK	.00	4:21pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

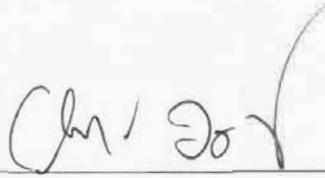

Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 02 480

Serial Number: 008970 Test Record Number: 752
Test Date: 08/22/2020 Test Time: 4:22pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:23pm
FLO	Pass	4:23pm
FC	Pass	4:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:23pm
SRC	Pass	4:23pm
DET	Pass	4:23pm
BAR	Pass	4:23pm
BT	Pass	4:23pm

Blank Tests

Test	Status	Time
AIR	Pass	4:24pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:24pm

CRC Tests

Test	Status	Time
COMP	Pass	4:24pm
CAL	Pass	4:24pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Fredell Instrument Location Dist mobile unit 2

Instrument Serial No. 006973 Wildfire

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Ch v Jof

Signature of Certifying Official

658

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 02 480

Serial Number: 008973
Test Date: 08/22/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: TOWERY, CHAD V
Permit Number: 26632E
Effective:
05/01/2019-05/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG902201
Exp Date: 01/22/2021


Test	g/210L	Time
DIAG	Pass	4:14pm
AIR BLK	.00	4:15pm
ACCY CHK	.08	4:16pm
AIR BLK	.00	4:16pm
SUB TEST	.00	4:17pm
AIR BLK	.00	4:18pm
SUB TEST	.00	4:19pm
AIR BLK	.00	4:20pm

Reported AC: .00 g/210L

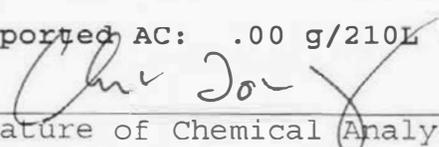

Signature of Chemical Analyst

Court CVR

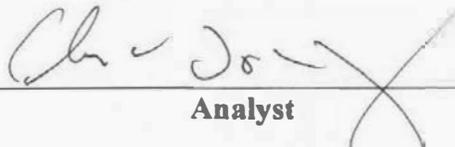

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 02 480

Serial Number: 008973 Test Record Number: 825
Test Date: 08/22/2020 Test Time: 4:21pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:21pm
FLO	Pass	4:21pm
FC	Pass	4:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:22pm
SRC	Pass	4:22pm
DET	Pass	4:22pm
BAR	Pass	4:22pm
BT	Pass	4:22pm

Blank Tests

Test	Status	Time
AIR	Pass	4:22pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:22pm

CRC Tests

Test	Status	Time
COMP	Pass	4:22pm
CAL	Pass	4:22pm

Preventive Maintenance
Status: Pass

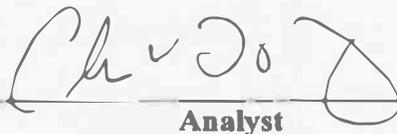

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County LEE Instrument Location SANFORD POLICE DEPT
Instrument Serial No. 008867 SANFORD, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5TH day of AUGUST, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]

Signature of Certifying Official

667

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LEE COUNTY SANFORD POLICE DEPT 520

Serial Number: 008867

Test Date: 08/05/2020

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

02/17/2020-02/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG934001

Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	4:18pm
AIR BLK	.00	4:19pm
ACCY CHK	.08	4:19pm
AIR BLK	.00	4:20pm
SUB TEST	.00	4:21pm
AIR BLK	.00	4:22pm
SUB TEST	.00	4:23pm
AIR BLK	.00	4:24pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

LEE COUNTY SANFORD POLICE DEPT 520

Serial Number: 008867 Test Record Number: 1168
Test Date: 08/05/2020 Test Time: 4:27pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:27pm
FLO	Pass	4:27pm
FC	Pass	4:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:27pm
SRC	Pass	4:27pm
DET	Pass	4:27pm
BAR	Pass	4:27pm
BT	Pass	4:27pm

Blank Tests

Test	Status	Time
AIR	Pass	4:28pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:28pm

CRC Tests

Test	Status	Time
COMP	Pass	4:28pm
CAL	Pass	4:28pm

Preventive Maintenance
Status: Pass

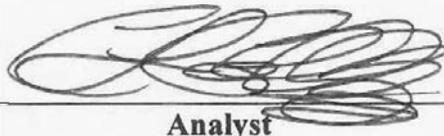

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAF Mobile Unit 2
Instrument Serial No. 008973 CM7D

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Chris Doy

Signature of Certifying Official

658

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 02
590

Serial Number: 008973
Test Date: 08/12/2020

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: TOWERY, CHAD V

Permit Number: 26632E

Effective:

05/01/2019-05/01/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG902201

Exp Date: 01/22/2021


Test	g/210L	Time
DIAG	Pass	7:51pm
AIR BLK	.00	7:52pm
ACCY CHK	.08	7:53pm
AIR BLK	.00	7:54pm
SUB TEST	.00	7:54pm
AIR BLK	.00	7:55pm
SUB TEST	.00	7:57pm
AIR BLK	.00	7:58pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 02 590

Serial Number: 008973 Test Record Number: 821
Test Date: 08/12/2020 Test Time: 7:59pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:59pm
FLO	Pass	7:59pm
FC	Pass	7:59pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:59pm
SRC	Pass	7:59pm
DET	Pass	7:59pm
BAR	Pass	7:59pm
BT	Pass	7:59pm

Blank Tests

Test	Status	Time
AIR	Pass	8:00pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:00pm

CRC Tests

Test	Status	Time
COMP	Pass	8:00pm
CAL	Pass	8:00pm

Preventive Maintenance
Status: Pass

Ch - 200

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 2

Instrument Serial No. 008970 CMFD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Chris-Joy

Signature of Certifying Official

658

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 02
590

Serial Number: 008970
Test Date: 08/12/2020

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: TOWERY, CHAD V

Permit Number: 26632E

Effective:

05/01/2019-05/01/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG902201

Exp Date: 01/22/2021


Test	g/210L	Time
DIAG	Pass	7:53pm
AIR BLK	.00	7:54pm
ACCY CHK	.08	7:55pm
AIR BLK	.00	7:56pm
SUB TEST	.00	7:56pm
AIR BLK	.00	7:57pm
SUB TEST	.00	7:59pm
AIR BLK	.00	7:59pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 02 590

Serial Number: 008970 Test Record Number: 745
Test Date: 08/12/2020 Test Time: 8:00pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:00pm
FLO	Pass	8:00pm
FC	Pass	8:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:01pm
SRC	Pass	8:01pm
DET	Pass	8:01pm
BAR	Pass	8:01pm
BT	Pass	8:01pm

Blank Tests

Test	Status	Time
AIR	Pass	8:01pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:01pm

CRC Tests

Test	Status	Time
COMP	Pass	8:01pm
CAL	Pass	8:01pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mitchell Instrument Location Spruce Pine Police Dept.

Instrument Serial No. 008736 Spruce Pine, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MITCHELL COUNTY SPRUCE PINE PD 600

Serial Number: 008726
Test Date: 08/03/2020

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XK

Driver's License Number: NONE

Analyst's Name: LOFTIS, BENJAMIN C

Permit Number: 24801E

Effective:

07/01/2019-07/01/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG920301


Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	9:47am
AIR BLK	.00	9:48am
ACCY CHK	.08	9:49am
AIR BLK	.00	9:50am
SUB TEST	.00	9:50am
AIR BLK	.00	9:52am
SUB TEST	.00	9:53am
AIR BLK	.00	9:54am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

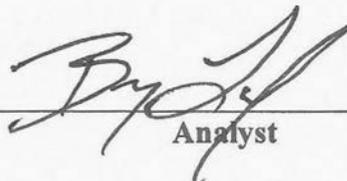
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MITCHELL COUNTY SPRUCE PINE PD 500

Serial Number: 008726 Test Record Number: 1052
Test Date: 08/03/2020 Test Time: 9:54am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:55am
FLO	Pass	9:55am
FC	Pass	9:55am

Temperature Tests

Test	Status	Time
FCL	Pass	9:55am
SRC	Pass	9:55am
DET	Pass	9:55am
BAE	Pass	9:55am
BT	Pass	9:55am

Blank Tests

Test	Status	Time
AIR	Pass	9:56am


Printer Tests

Test	Status	Time
PRNT	Pass	9:56am

CRC Tests

Test	Status	Time
COMP	Pass	9:56am
CAL	Pass	9:56am

Preventive Maintenance
Status: Pass

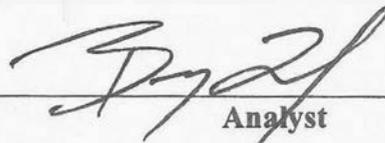

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County MOORE Instrument Location MOORE CO. DETENTION CENTER
Instrument Serial No. 008735 CARTHAGE, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17TH day of AUGUST, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Signature of Certifying Official

667

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MOORE COUNTY DETENTION CENTER 620

Serial Number: 008735
Test Date: 08/17/2020

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

02/17/2020-02/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG933703

Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	5:53pm
AIR BLK	.00	5:54pm
ACCY CHK	.08	5:54pm
AIR BLK	.00	5:55pm
SUB TEST	.00	5:56pm
AIR BLK	.00	5:57pm
SUB TEST	.00	5:59pm
AIR BLK	.00	5:59pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MOORE COUNTY DETENTION CENTER 620

Serial Number: 008735 Test Record Number: 2454
Test Date: 08/17/2020 Test Time: 6:00pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:01pm
FLO	Pass	6:01pm
FC	Pass	6:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:01pm
SRC	Pass	6:01pm
DET	Pass	6:01pm
BAR	Pass	6:01pm
BT	Pass	6:01pm

Blank Tests

Test	Status	Time
AIR	Pass	6:02pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:02pm

CRC Tests

Test	Status	Time
COMP	Pass	6:02pm
CAL	Pass	6:02pm

Preventive Maintenance
Status: Pass

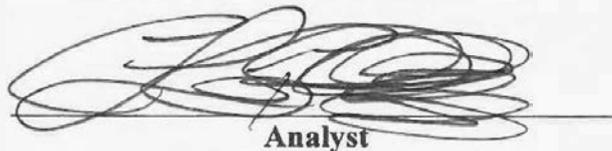

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County WASH Instrument Location NASHVILLE PD
Instrument Serial No. 008630 501 S. BARNES ST NASHVILLE, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

62
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY NASHVILLE PD 630

Serial Number: 008630
Test Date: 08/05/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, STOKES
Permit Number: 11434E
Effective:
04/01/2019-04/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022


Test	g/210L	Time
DIAG	Pass	9:48am
AIR BLK	.00	9:49am
ACCY CHK	.08	9:50am
AIR BLK	.00	9:51am
SUB TEST	.00	9:51am
AIR BLK	.00	9:52am
SUB TEST	.00	9:53am
AIR BLK	.00	9:54am

Reported AC: .00 g/210L

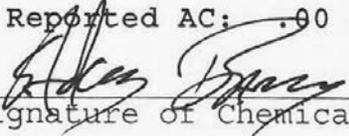

Signature of Chemical Analyst

Court CVR

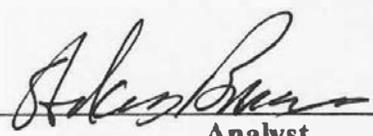

Analyst

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY NASHVILLE PD 630

Serial Number: 008630 Test Record Number: 4838
Test Date: 08/05/2020 Test Time: 9:55am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:55am
FLO	Pass	9:55am
FC	Pass	9:55am

Temperature Tests

Test	Status	Time
FC1	Pass	9:55am
SRC	Pass	9:55am
DET	Pass	9:55am
BAR	Pass	9:55am
BT	Pass	9:55am

Blank Tests

Test	Status	Time
AIR	Pass	9:56am


Printer Tests

Test	Status	Time
PRNT	Pass	9:56am

CRC Tests

Test	Status	Time
COMP	Pass	9:56am
CAL	Pass	9:56am

Preventive Maintenance
Status: Pass

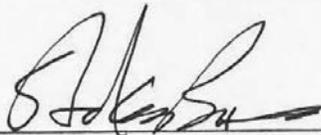

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County NASH Instrument Location Rocky Mount PD

Instrument Serial No. 008740 #1 Government PLAZA Rocky Mount, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Stokes Barnes 662
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY ROCKY MOUNT PD 630

Serial Number: 008740

Test Date: 08/05/2020

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, STOKES

Permit Number: 11434E

Effective:

04/01/2019-04/01/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG919902

Exp Date: 07/18/2021


Test	g/210L	Time
DIAG	Pass	8:39am
AIR BLK	.00	8:40am
ACCY CHK	.07	8:40am
AIR BLK	.00	8:41am
SUB TEST	.00	8:42am
AIR BLK	.00	8:43am
SUB TEST	.00	8:44am
AIR BLK	.00	8:45am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

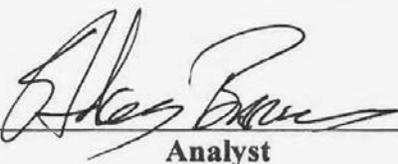

Analyst

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY ROCKY MOUNT PD 630

Serial Number: 008740 Test Record Number: 746
Test Date: 08/05/2020 Test Time: 8:47am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:48am
FLO	Pass	8:48am
FC	Pass	8:48am

Temperature Tests

Test	Status	Time
FC1	Pass	8:48am
SRC	Pass	8:48am
DET	Pass	8:48am
BAR	Pass	8:48am
BT	Pass	8:48am

Blank Tests

Test	Status	Time
AIR	Pass	8:49am


Printer Tests

Test	Status	Time
PRNT	Pass	8:49am

CRC Tests

Test	Status	Time
COMP	Pass	8:49am
CAL	Pass	8:49am

Preventive Maintenance
Status: Pass

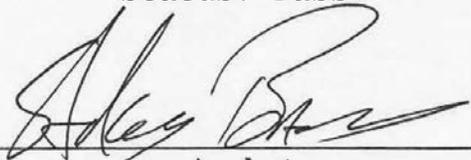

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County NASH Instrument Location Rocky Mount PD

Instrument Serial No. DD 8741 #1 Government Plaza Rocky Mount, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alex Bruns

Signature of Certifying Official

662

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY ROCKY MOUNT PD 630

Serial Number: 008741
Test Date: 08/05/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, STOKES
Permit Number: 11434E
Effective:
04/01/2019-04/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG919902
Exp Date: 07/18/2021


Test	g/210L	Time
DIAG	Pass	8:39am
AIR BLK	.00	8:40am
ACCY CHK	.07	8:41am
AIR BLK	.00	8:42am
SUB TEST	.00	8:42am
AIR BLK	.00	8:43am
SUB TEST	.00	8:45am
AIR BLK	.00	8:45am

Reported AC: .00 g/210L

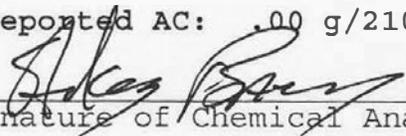

Signature of Chemical Analyst

Court CVR

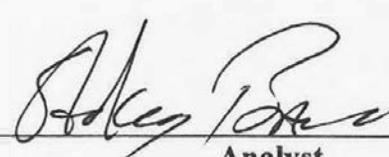

Analyst

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY ROCKY MOUNT PD 630

Serial Number: 008741 Test Record Number: 2617
Test Date: 08/05/2020 Test Time: 8:48am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	8:48am
FLO	Pass	8:48am
FC	Pass	8:48am

Temperature Tests

Test	Status	Time
FC1	Pass	8:48am
SRC	Pass	8:48am
DET	Pass	8:48am
BAR	Pass	8:48am
BT	Pass	8:48am

Blank Tests

Test	Status	Time
AIR	Pass	8:49am


Printer Tests

Test	Status	Time
PRNT	Pass	8:49am

CRC Tests

Test	Status	Time
COMP	Pass	8:49am
CAL	Pass	8:49am

Preventive Maintenance
Status: Pass

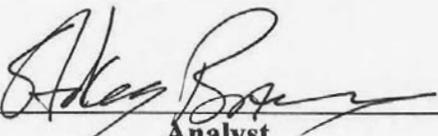
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Northampton Instrument Location Northampton Co. S.O.

Instrument Serial No. 008607 105 W. Jefferson St. Jackson, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Stokes Brown
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

**NORTHAMPTON COUNTY SHERIFFS DEPARTMENT
650**

Serial Number: 008607
Test Date: 08/05/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: *BARNES, STOKES*
Permit Number: 11434E
Effective:
04/01/2019-04/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG919902
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	12:53pm
AIR BLK	.00	12:53pm
ACCY CHK	.07	12:54pm
AIR BLK	.00	12:55pm
SUB TEST	.00	12:56pm
AIR BLK	.00	12:57pm
SUB TEST	.00	12:58pm
AIR BLK	.00	12:59pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

NORTHAMPTON COUNTY SHERIFFS DEPARTMENT 650

Serial Number: 008607 Test Record Number: 1051
Test Date: 08/05/2020 Test Time: 1:00pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:00pm
FLO	Pass	1:00pm
FC	Pass	1:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:00pm
SRC	Pass	1:00pm
DET	Pass	1:00pm
BAR	Pass	1:00pm
BT	Pass	1:00pm

Blank Tests

Test	Status	Time
AIR	Pass	1:01pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:01pm

CRC Tests

Test	Status	Time
COMP	Pass	1:01pm
CAL	Pass	1:01pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Northampton Instrument Location Northampton Co. S.O.
Instrument Serial No. 008288 105 W. Jefferson St. Jackson, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

662

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NORTHAMPTON COUNTY SHERIFFS DEPARTMENT
650

Serial Number: 008688
Test Date: 08/05/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, STOKES
Permit Number: 11434E
Effective:
04/01/2019-04/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG919902
Exp Date: 07/18/2021


Test	g/210L	Time
DIAG	Pass	12:54pm
AIR BLK	.00	12:54pm
ACCY CHK	.07	12:55pm
AIR BLK	.00	12:56pm
SUB TEST	.00	12:56pm
AIR BLK	.00	12:57pm
SUB TEST	.00	12:59pm
AIR BLK	.00	1:00pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

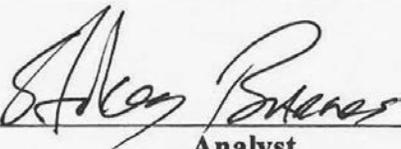

Analyst

Intox EC/IR-II: Preventive Maintenance

NORTHAMPTON COUNTY SHERIFFS DEPARTMENT 650

Serial Number: 008688 Test Record Number: 879
Test Date: 08/05/2020 Test Time: 1:01pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:01pm
FLO	Pass	1:01pm
FC	Pass	1:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:01pm
SRC	Pass	1:01pm
DET	Pass	1:01pm
BAR	Pass	1:01pm
BT	Pass	1:01pm

Blank Tests

Test	Status	Time
AIR	Pass	1:02pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:02pm

CRC Tests

Test	Status	Time
COMP	Pass	1:02pm
CAL	Pass	1:02pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Onslow Instrument Location BAT mobile unit #5
Instrument Serial No. 008707 North Topsail PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

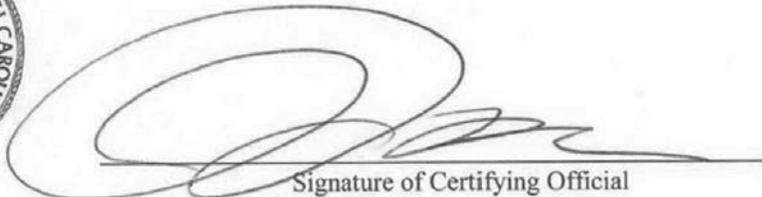


Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE UNIT 5 660

Serial Number: 008707
Test Date: 08/20/2020

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Todd, Shane C

Permit Number: 0035-4789

Effective:

06/08/2020-06/08/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG919902

Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	3:17pm
AIR BLK	.00	3:18pm
ACCY CHK	.08	3:19pm
AIR BLK	.00	3:19pm
SUB TEST	.00	3:20pm
AIR BLK	.00	3:21pm
SUB TEST	.00	3:22pm
AIR BLK	.00	3:23pm

Reported AC: .00 g/210L

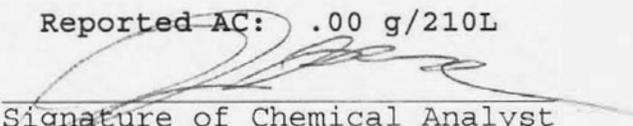
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 5 660

Serial Number: 008707 Test Record Number: 2645
Test Date: 08/20/2020 Test Time: 3:24pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:24pm
FLO	Pass	3:24pm
FC	Pass	3:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:25pm
SRC	Pass	3:25pm
DET	Pass	3:25pm
BAR	Pass	3:25pm
BT	Pass	3:25pm

Blank Tests

Test	Status	Time
AIR	Pass	3:25pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:25pm

CRC Tests

Test	Status	Time
COMP	Pass	3:25pm
CAL	Pass	3:25pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Onslow Instrument Location DAT Mobile Unit 12

Instrument Serial No. 008600 Sneads Ferry

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

665

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE 12 660

Serial Number: 008600
Test Date: 08/08 2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Anderson, Mark G
Permit Number: 0013-1517
Effective:
09/23/2019-09/23/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG919902
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	10:55pm
AIR BLK	.00	10:56pm
ACCY CHK	.07	10:56pm
AIR BLK	.00	10:57pm
SUB TEST	.00	11:01pm
AIR BLK	.00	11:01pm
SUB TEST	.00	11:03pm
AIR BLK	.00	11:04pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE 12 660

Serial Number: 008600 Test Record Number: 1981
Test Date: 08/08/2020 Test Time: 11:08pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:09pm
FLO	Pass	11:09pm
FC	Pass	11:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:09pm
SRC	Pass	11:09pm
DET	Pass	11:09pm
BAR	Pass	11:09pm
BT	Pass	11:09pm

Blank Tests

Test	Status	Time
AIR	Pass	11:10pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:10pm

CRC Tests

Test	Status	Time
COMP	Pass	11:10pm
CAL	Pass	11:10pm

Preventive Maintenance
Status: Pass

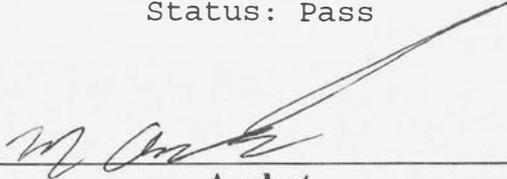

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Onslow Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008600 Jacksonville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

665
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ON SLOW COUNTY BAT MOBILE 12 660

Serial Number: 008600
Test Date: 08/12/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Anderson, Mark G
Permit Number: 0013-1517
Effective:
09/23/2019-09/23/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG919902
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	10:38pm
AIR BLK	.00	10:39pm
ACCY CHK	.08	10:40pm
AIR BLK	.00	10:41pm
SUB TEST	.00	10:41pm
AIR BLK	.00	10:42pm
SUB TEST	.00	10:44pm
AIR BLK	.00	10:45pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE 12 660

Serial Number: 008600 Test Record Number: 1984
Test Date: 08/12/2020 Test Time: 10:46pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:47pm
FLO	Pass	10:47pm
FC	Pass	10:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:47pm
SRC	Pass	10:47pm
DET	Pass	10:47pm
BAR	Pass	10:47pm
BT	Pass	10:47pm

Blank Tests

Test	Status	Time
AIR	Pass	10:47pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:48pm

CRC Tests

Test	Status	Time
COMP	Pass	10:48pm
CAL	Pass	10:48pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Onslow Instrument Location BAT mobile unit 12

Instrument Serial No. 008698 swansboro

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

665
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE 12 660

Serial Number: 008698
Test Date: 08/13/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Anderson, Mark G
Permit Number: 0013-1517
Effective:
09/23/2019-09/23/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	6:24pm
AIR BLK	.00	6:25pm
ACCY CHK	.08	6:26pm
AIR BLK	.00	6:26pm
SUB TEST	.00	6:27pm
AIR BLK	.00	6:28pm
SUB TEST	.00	6:29pm
AIR BLK	.00	6:30pm

Reported AC: 00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE 12 660

Serial Number: 008698 Test Record Number: 1565
Test Date: 08/13/2020 Test Time: 6:39pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:39pm
FLO	Pass	6:39pm
FC	Pass	6:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:40pm
SRC	Pass	6:40pm
DET	Pass	6:40pm
BAR	Pass	6:40pm
BT	Pass	6:40pm

Blank Tests

Test	Status	Time
AIR	Pass	6:40pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:40pm

CRC Tests

Test	Status	Time
COMP	Pass	6:41pm
CAL	Pass	6:41pm

Preventive Maintenance
Status: Pass

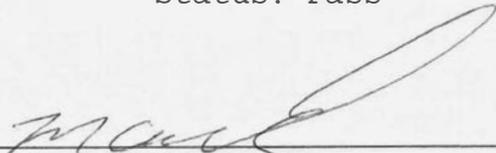

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Onslow Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008788 Jacksonville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

665

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE UNIT 12 660

Serial Number: 008788
Test Date: 08/12/2020

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Anderson, Mark G

Permit Number: 0013-1517

Effective:

09/23/2019-09/23/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG911506

Exp Date: 04/25/2021

Test	g/210L	Time
DIAG	Pass	10:21pm
AIR BLK	.00	10:22pm
ACCY CHK	.08	10:23pm
AIR BLK	.00	10:24pm
SUB TEST	.00	10:24pm
AIR BLK	.00	10:25pm
SUB TEST	.00	10:27pm
AIR BLK	.00	10:28pm

Reported AC: .00 g/210L

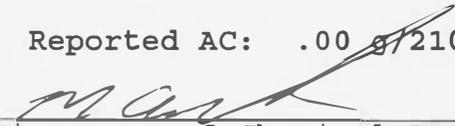

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE UNIT 12 660

Serial Number: 008788 Test Record Number: 1546
Test Date: 08/12/2020 Test Time: 10:29pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:29pm
FLO	Pass	10:29pm
FC	Pass	10:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:29pm
SRC	Pass	10:29pm
DET	Pass	10:29pm
BAR	Pass	10:29pm
BT	Pass	10:29pm

Blank Tests

Test	Status	Time
AIR	Pass	10:30pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:30pm

CRC Tests

Test	Status	Time
COMP	Pass	10:30pm
CAL	Pass	10:30pm

Preventive Maintenance
Status: Pass

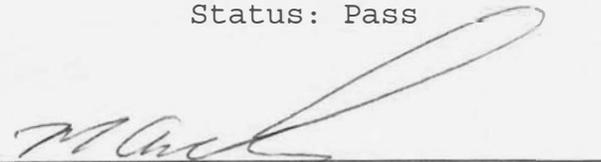

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Onslow Instrument Location MCAS New River
Instrument Serial No. 008919 PMO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of August, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. B...
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY MCAS NEW RIVER 660

Serial Number: 008919

Test Date: 08/20/2020

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 15671E

Effective:

06/01/2019-06/01/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG934001


Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	10:28am
AIR BLK	.00	10:28am
ACCY CHK	.08	10:29am
AIR BLK	.00	10:30am
SUB TEST	.00	10:31am
AIR BLK	.00	10:31am
SUB TEST	.00	10:33am
AIR BLK	.00	10:34am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY MCAS NEW RIVER 660

Serial Number: 008919 Test Record Number: 685
Test Date: 08/20/2020 Test Time: 10:35am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:35am
FLO	Pass	10:35am
FC	Pass	10:36am

Temperature Tests

Test	Status	Time
FC1	Pass	10:36am
SRC	Pass	10:36am
DET	Pass	10:36am
BAR	Pass	10:36am
BT	Pass	10:36am

Blank Tests

Test	Status	Time
AIR	Pass	10:36am


Printer Tests

Test	Status	Time
PRNT	Pass	10:36am

CRC Tests

Test	Status	Time
COMP	Pass	10:36am
CAL	Pass	10:36am

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONSLow Instrument Location CAMP LEJEUNE
Instrument Serial No. 008920 PMO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of AUGUST, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Bowers
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY CAMP LEJEUNE PMO 660

Serial Number: 008920
Test Date: 08/19/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 15671E
Effective:
06/01/2019-06/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG018801
Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	3:41pm
AIR BLK	.00	3:41pm
ACCY CHK	.08	3:42pm
AIR BLK	.00	3:43pm
SUB TEST	.00	3:43pm
AIR BLK	.00	3:44pm
SUB TEST	.00	3:46pm
AIR BLK	.00	3:46pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY CAMP LEJEUNE PMO 660

Serial Number: 008920 Test Record Number: 1844
Test Date: 08/19/2020 Test Time: 3:49pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:49pm
FLO	Pass	3:49pm
FC	Pass	3:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:49pm
SRC	Pass	3:49pm
DET	Pass	3:49pm
BAR	Pass	3:49pm
BT	Pass	3:49pm

Blank Tests

Test	Status	Time
AIR	Pass	3:50pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:50pm

CRC Tests

Test	Status	Time
COMP	Pass	3:50pm
CAL	Pass	3:50pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County ONslow Instrument Location JACKSONVILLE
Instrument Serial No. 008930 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of AUGUST, 2020, the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Benson
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY JACKSONVILLE PD 660

Serial Number: 008930
Test Date: 08/19/2020

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 15671E

Effective:

06/01/2019-06/01/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG018801


Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	2:19pm
AIR BLK	.00	2:19pm
ACCY CHK	.08	2:20pm
AIR BLK	.00	2:21pm
SUB TEST	.00	2:21pm
AIR BLK	.00	2:22pm
SUB TEST	.00	2:24pm
AIR BLK	.00	2:25pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY JACKSONVILLE PD 660

Serial Number: 008930 Test Record Number: 2083
Test Date: 08/19/2020 Test Time: 2:26pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:26pm
FLO	Pass	2:26pm
FC	Pass	2:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:26pm
SRC	Pass	2:26pm
DET	Pass	2:26pm
BAR	Pass	2:26pm
BT	Pass	2:26pm

Blank Tests

Test	Status	Time
AIR	Pass	2:27pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:27pm

CRC Tests

Test	Status	Time
COMP	Pass	2:27pm
CAL	Pass	2:27pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ONSHLOW Instrument Location ONSHLOW COUNTY
Instrument Serial No. 008931 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of AUGUST, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Basso

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY DETENTION CENTER 660

Serial Number: 008931
Test Date: 08/19/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 15671E
Effective:
06/01/2019-06/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG018801
Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	11:16am
AIR BLK	.00	11:16am
ACCY CHK	.08	11:17am
AIR BLK	.00	11:18am
SUB TEST	.00	11:19am
AIR BLK	.00	11:20am
SUB TEST	.00	11:21am
AIR BLK	.00	11:22am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY DETENTION CENTER 660

Serial Number: 008931 Test Record Number: 3376
Test Date: 08/19/2020 Test Time: 11:24am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:24am
FLO	Pass	11:24am
FC	Pass	11:24am

Temperature Tests

Test	Status	Time
FC1	Pass	11:24am
SRC	Pass	11:24am
DET	Pass	11:24am
BAR	Pass	11:24am
BT	Pass	11:24am

Blank Tests

Test	Status	Time
AIR	Pass	11:25am


Printer Tests

Test	Status	Time
PRNT	Pass	11:25am

CRC Tests

Test	Status	Time
COMP	Pass	11:25am
CAL	Pass	11:25am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ONSLOW Instrument Location ONSLOW COUNTY
Instrument Serial No. 008932 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of AUGUST, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan Rg Baus

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY DETENTION CENTER 660

Serial Number: 008932
Test Date: 08/19/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 15671E
Effective:
06/01/2019-06/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG018801
Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	11:54am
AIR BLK	.00	11:55am
ACCY CHK	.08	11:55am
AIR BLK	.00	11:57am
SUB TEST	.00	11:57am
AIR BLK	.00	11:58am
SUB TEST	.00	12:00pm
AIR BLK	.00	12:01pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY DETENTION CENTER 660

Serial Number: 008932 Test Record Number: 5649
Test Date: 08/19/2020 Test Time: 12:02pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:02pm
FLO	Pass	12:02pm
FC	Pass	12:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:03pm
SRC	Pass	12:03pm
DET	Pass	12:03pm
BAR	Pass	12:03pm
BT	Pass	12:03pm

Blank Tests

Test	Status	Time
AIR	Pass	12:03pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:03pm

CRC Tests

Test	Status	Time
COMP	Pass	12:04pm
CAL	Pass	12:04pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Person Instrument Location Person Co IEC
Instrument Serial No. 008693 120 Court St Roxboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PERSON COUNTY PERSON CO. LEC 720

Serial Number: 008693
Test Date: 08/03/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, STOKES
Permit Number: 11434E
Effective:
04/01/2019-04/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018401
Exp Date: 07/02/2022


Test	g/210L	Time
DIAG	Pass	7:52am
AIR BLK	.00	7:54am
ACCY CHK	.07	7:54am
AIR BLK	.00	7:55am
SUB TEST	.00	7:56am
AIR BLK	.00	7:57am
SUB TEST	.00	7:59am
AIR BLK	.00	7:59am

Reported AC: .00 g/210L

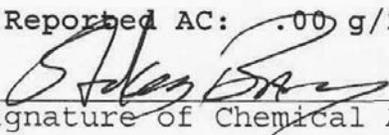

Signature of Chemical Analyst

Court CVR

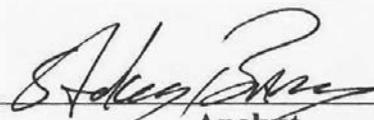

Analyst

Intox EC/IR-II: Preventive Maintenance

PERSON COUNTY PERSON CO. LEC 720

Serial Number: 008693 Test Record Number: 1716
Test Date: 08/03/2020 Test Time: 8:00am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:01am
FLO	Pass	8:01am
FC	Pass	8:01am

Temperature Tests

Test	Status	Time
FC1	Pass	8:01am
SRC	Pass	8:01am
DET	Pass	8:01am
BAR	Pass	8:01am
BT	Pass	8:01am

Blank Tests

Test	Status	Time
AIR	Pass	8:01am

Printer Tests

Test	Status	Time
PRNT	Pass	8:01am

CRC Tests

Test	Status	Time
COMP	Pass	8:02am
CAL	Pass	8:02am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Person Instrument Location Person Co LEC

Instrument Serial No. 008880 120 Court St. Roxboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alex Barnes

Signature of Certifying Official

642

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PERSON COUNTY PERSON CO. LEC 720

Serial Number: 008880
Test Date: 08/03/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, STOKES
Permit Number: 11434E
Effective:
04/01/2019-04/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018401
Exp Date: 07/02/2022


Test	g/210L	Time
DIAG	Pass	7:52am
AIR BLK	.00	7:53am
ACCY CHK	.08	7:53am
AIR BLK	.00	7:54am
SUB TEST	.00	7:55am
AIR BLK	.00	7:56am
SUB TEST	.00	7:57am
AIR BLK	.00	7:58am

Reported AC: .00 g/210L

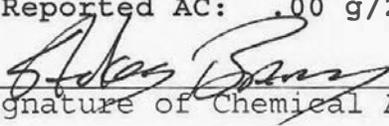

Signature of Chemical Analyst

Court CVR

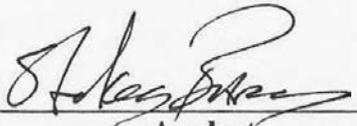

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

PERSON COUNTY PERSON CO. LEC 720

Serial Number: 008880 Test Record Number: 1635
Test Date: 08/03/2020 Test Time: 8:00am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:00am
FLO	Pass	8:00am
FC	Pass	8:00am

Temperature Tests

Test	Status	Time
FC1	Pass	8:01am
SRC	Pass	8:01am
DET	Pass	8:01am
BAR	Pass	8:01am
BT	Pass	8:01am

Blank Tests

Test	Status	Time
AIR	Pass	8:01am


Printer Tests

Test	Status	Time
PRNT	Pass	8:01am

CRC Tests

Test	Status	Time
COMP	Pass	8:01am
CAL	Pass	8:01am

Preventive Maintenance
Status: Pass

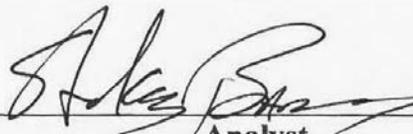

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Pitt Instrument Location Pitt Co. Detention Center
Instrument Serial No. 008646 124 New Hope Rd., Greenville,
N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of AUGUST, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008646
Test Date: 08/06/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Keesler, Linda A
Permit Number: 0045-5468
Effective:
07/08/2019-07/08/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG902201
Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	4:07pm
AIR BLK	.00	4:07pm
ACCY CHK	.08	4:08pm
AIR BLK	.00	4:09pm
SUB TEST	.00	4:11pm
AIR BLK	.00	4:12pm
SUB TEST	.00	4:14pm
AIR BLK	.00	4:15pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008646 Test Record Number: 4047
Test Date: 08/06/2020 Test Time: 4:15pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:15pm
FLO	Pass	4:15pm
FC	Pass	4:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:16pm
SRC	Pass	4:16pm
DET	Pass	4:16pm
BAR	Pass	4:16pm
BT	Pass	4:16pm

Blank Tests

Test	Status	Time
AIR	Pass	4:16pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:16pm

CRC Tests

Test	Status	Time
COMP	Pass	4:16pm
CAL	Pass	4:16pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County PITT Instrument Location Pitt co. Detention Center
Instrument Serial No. 008662 124 New Hope Rd., Roseville, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of AUGUST, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008662
Test Date: 08/06/2020

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Keesler, Linda A

Permit Number: 0045-5468

Effective:

07/08/2019-07/08/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG902201

Exp Date: 01/22/2021

Test	g/210L	Time
DIAG	Pass	4:11pm
AIR BLK	.00	4:11pm
ACCY CHK	.08	4:12pm
AIR BLK	.00	4:13pm
SUB TEST	.00	4:14pm
AIR BLK	.00	4:15pm
SUB TEST	.00	4:17pm
AIR BLK	.00	4:18pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008662 Test Record Number: 1177
Test Date: 08/06/2020 Test Time: 4:18pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:19pm
FLO	Pass	4:19pm
FC	Pass	4:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:19pm
SRC	Pass	4:19pm
DET	Pass	4:19pm
BAR	Pass	4:19pm
BT	Pass	4:19pm

Blank Tests

Test	Status	Time
AIR	Pass	4:20pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:20pm

CRC Tests

Test	Status	Time
COMP	Pass	4:20pm
CAL	Pass	4:20pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Pitt Instrument Location Pitt Co. Detention Center
Instrument Serial No. 008668 124 New Hope Rd., Greenville
NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Linna Kees
Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008668

Test Date: 08/06/2020

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Keesler, Linda A

Permit Number: 0045-5468

Effective:

07/08/2019-07/08/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG920301


Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	11:07am
AIR BLK	.00	11:07am
ACCY CHK	.08	11:08am
AIR BLK	.00	11:09am
SUB TEST	.00	11:09am
AIR BLK	.00	11:11am
SUB TEST	.00	11:12am
AIR BLK	.00	11:13am

Reported AC: 00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008668 Test Record Number: 3657
Test Date: 08/06/2020 Test Time: 11:13am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:14am
FLO	Pass	11:14am
FC	Pass	11:14am

Temperature Tests

Test	Status	Time
FC1	Pass	11:14am
SRC	Pass	11:14am
DET	Pass	11:14am
BAR	Pass	11:14am
BT	Pass	11:14am

Blank Tests

Test	Status	Time
AIR	Pass	11:15am


Printer Tests

Test	Status	Time
PRNT	Pass	11:15am

CRC Tests

Test	Status	Time
COMP	Pass	11:15am
CAL	Pass	11:15am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Robeson Instrument Location BAT Mobile Unit #5
Instrument Serial No. 008704 Robeson Co. S.D.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

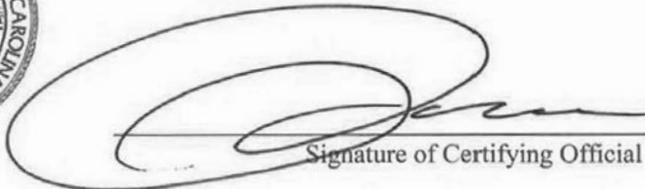


Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008704
Test Date: 08/02/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Todd, Shane C
Permit Number: 0035-4789
Effective:
06/08/2020-06/08/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG807101
Exp Date: 12/03/2021


Test	g/210L	Time
DIAG	Pass	7:41pm
AIR BLK	.00	7:42pm
ACCY CHK	.08	7:42pm
AIR BLK	.00	7:43pm
SUB TEST	.00	7:44pm
AIR BLK	.00	7:45pm
SUB TEST	.00	7:46pm
AIR BLK	.00	7:47pm

Reported AC: .00 g/210L

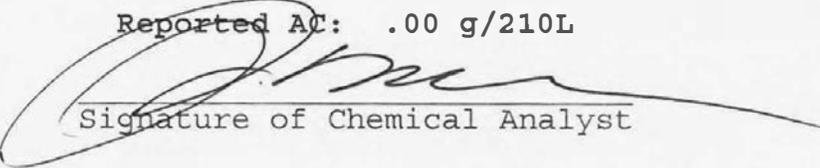

Signature of Chemical Analyst

Court CVR

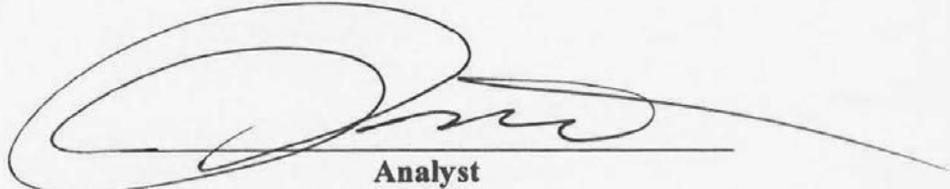

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008704 Test Record Number: 652
Test Date: 08/02/2020 Test Time: 7:50pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:50pm
FLO	Pass	7:50pm
FC	Pass	7:50pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:50pm
SRC	Pass	7:50pm
DET	Pass	7:50pm
BAR	Pass	7:50pm
BT	Pass	7:50pm

Blank Tests

Test	Status	Time
AIR	Pass	7:51pm


Printer Tests

Test	Status	Time
PRNT	Pass	7:51pm

CRC Tests

Test	Status	Time
COMP	Pass	7:51pm
CAL	Pass	7:51pm

Preventive Maintenance
Status: Pass

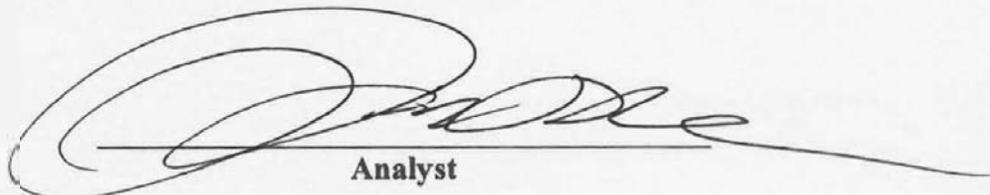

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Stanly Instrument Location Locust PD

Instrument Serial No. 008706

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official
656 Certificate Number

Intox EC/IR-II: Subject Test

STANLY LOCUST PD 830

Serial Number: 008706

Test Date: 08/13/2020

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hays, Mark D

Permit Number: 0011-3099

Effective:

11/13/2019-11/13/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG933901

Exp Date: 12/05/2021


Test	g/210L	Time
DIAG	Pass	9:32am
AIR BLK	.00	9:33am
ACCY CHK	.08	9:33am
AIR BLK	.00	9:34am
SUB TEST	.00	9:35am
AIR BLK	.00	9:36am
SUB TEST	.00	9:37am
AIR BLK	.00	9:38am

Reported AC: .00 g/210L

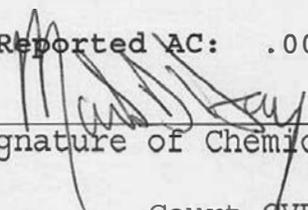

Signature of Chemical Analyst

Court CVR

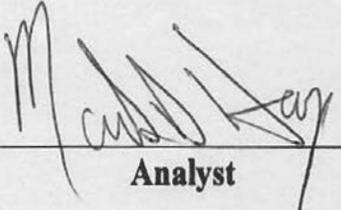

Analyst

Intox EC/IR-II: Preventive Maintenance

STANLY LOCUST PD 830

Serial Number: 008706 Test Record Number: 3559
Test Date: 08/13/2020 Test Time: 9:40am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:40am
FLO	Pass	9:40am
FC	Pass	9:40am

Temperature Tests

Test	Status	Time
FC1	Pass	9:40am
SRC	Pass	9:40am
DET	Pass	9:40am
BAR	Pass	9:40am
BT	Pass	9:40am

Blank Tests

Test	Status	Time
AIR	Pass	9:41am


Printer Tests

Test	Status	Time
PRNT	Pass	9:41am

CRC Tests

Test	Status	Time
COMP	Pass	9:41am
CAL	Pass	9:41am

Preventive Maintenance
Status: Pass

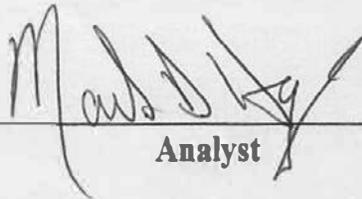

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Stanly Instrument Location Stanly County SO
Instrument Serial No. 008842

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



M. J. [Signature]
Signature of Certifying Official

656
Certificate Number

Intox EC/IR-II: Subject Test

STANLY COUNTY STANLY COUNTY SO 830

Serial Number: 008842
Test Date: 08/13/2020

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hays, Mark D

Permit Number: 0011-3099

Effective:

11/13/2019-11/13/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG919901

Exp Date: 07/18/2021


Test	g/210L	Time
DIAG	Pass	10:38am
AIR BLK	.00	10:39am
ACCY CHK	.08	10:39am
AIR BLK	.00	10:40am
SUB TEST	.00	10:42am
AIR BLK	.00	10:42am
SUB TEST	.00	10:45am
AIR BLK	.00	10:45am

Reported AC: .00 g/210L

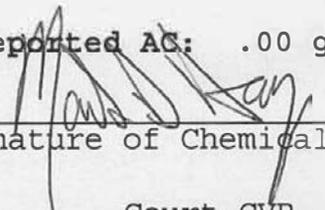

Signature of Chemical Analyst

Court CVR

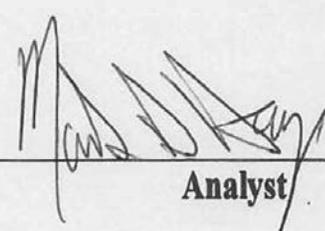

Analyst

Intox EC/IR-II: Preventive Maintenance

STANLY COUNTY STANLY COUNTY SO 830

Serial Number: 008842 Test Record Number: 2312
Test Date: 08/13/2020 Test Time: 10:48am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:48am
FLO	Pass	10:48am
FC	Pass	10:48am

Temperature Tests

Test	Status	Time
FC1	Pass	10:48am
SRC	Pass	10:48am
DET	Pass	10:48am
BAR	Pass	10:48am
BT	Pass	10:48am

Blank Tests

Test	Status	Time
AIR	Pass	10:49am


Printer Tests

Test	Status	Time
PRNT	Pass	10:49am

CRC Tests

Test	Status	Time
COMP	Pass	10:49am
CAL	Pass	10:49am

Preventive Maintenance
Status: Pass

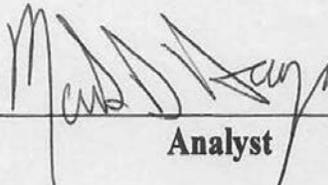

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Stokes Instrument Location Stokes Co Jail
Instrument Serial No. 008596 Danbury, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 649
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STOKES COUNTY STOKES COUNTY JAIL 340

Serial Number: 008596

Test Date: 08/11/2020

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J

Permit Number: 11304E

Effective:

06/01/2019-06/01/2021

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601


Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	6:49pm
AIR BLK	.00	6:50pm
ACCY CHK	.07	6:50pm
AIR BLK	.00	6:51pm
SUB TEST	.00	6:52pm
AIR BLK	.00	6:53pm
SUB TEST	.00	6:54pm
AIR BLK	.00	6:55pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

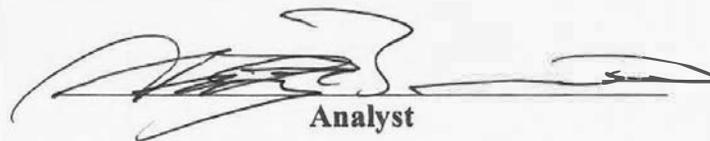

Analyst

Intox EC/IR-II: Preventive Maintenance

STOKES COUNTY STOKES COUNTY JAIL 840

Serial Number: 008596 Test Record Number: 1151
Test Date: 08/11/2020 Test Time: 6:56pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:57pm
FLO	Pass	6:57pm
FC	Pass	6:57pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:57pm
SRC	Pass	6:57pm
DET	Pass	6:57pm
BAR	Pass	6:57pm
BT	Pass	6:57pm

Blank Tests

Test	Status	Time
AIR	Pass	6:57pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:57pm

CRC Tests

Test	Status	Time
COMP	Pass	6:58pm
CAL	Pass	6:58pm

Preventive Maintenance
Status: Pass

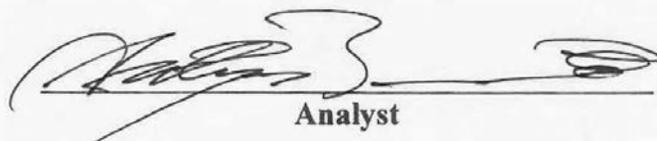
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Surry Instrument Location ELKIN

Instrument Serial No. 008926 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 649 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SURRY COUNTY ELKIN PD 850

Serial Number: 008926
Test Date: 08/31/2020

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J

Permit Number: 11304E

Effective:

06/01/2019-06/01/2021

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG920301

Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	2:48pm
AIR BLK	.00	2:49pm
ACCY CHK	.08	2:50pm
AIR BLK	.00	2:51pm
SUB TEST	.00	2:51pm
AIR BLK	.00	2:52pm
SUB TEST	.00	2:54pm
AIR BLK	.00	2:55pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY ELKIN PD 850

Serial Number: 008926 Test Record Number: 908
Test Date: 08/31/2020 Test Time: 2:58pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:58pm
FLO	Pass	2:58pm
FC	Pass	2:58pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:58pm
SRC	Pass	2:58pm
DET	Pass	2:58pm
BAR	Pass	2:58pm
BT	Pass	2:58pm

Blank Tests

Test	Status	Time
AIR	Pass	2:59pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:59pm

CRC Tests

Test	Status	Time
COMP	Pass	2:59pm
CAL	Pass	2:59pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Vance Instrument Location Vance Co S.O.

Instrument Serial No. 008870 156 Church St Henderson, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

VANCE COUNTY SHERIFF'S DEPARTMENT 900

Serial Number: 008870
Test Date: 08/04/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, STOKES
Permit Number: 11434E
Effective:
04/01/2019-04/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG911501
Exp Date: 04/25/2021


Test	g/210L	Time
DIAG	Pass	10:58am
AIR BLK	.00	10:59am
ACCY CHK	.08	10:59am
AIR BLK	.00	11:01am
SUB TEST	.00	11:02am
AIR BLK	.00	11:03am
SUB TEST	.00	11:04am
AIR BLK	.00	11:05am

Reported AC: .00 g/210L

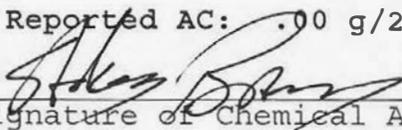

Signature of Chemical Analyst

Court CVR

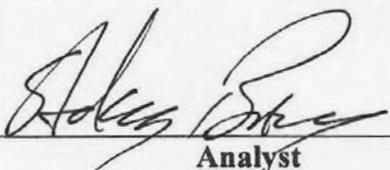

Analyst

Intox EC/IR-II: Preventive Maintenance

VANCE COUNTY SHERIFF'S DEPARTMENT 900

Serial Number: 008870 Test Record Number: 3046
Test Date: 08/04/2020 Test Time: 11:06am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:06am
FLO	Pass	11:06am
FC	Pass	11:06am

Temperature Tests

Test	Status	Time
FC1	Pass	11:06am
SRC	Pass	11:06am
DET	Pass	11:06am
BAR	Pass	11:06am
BT	Pass	11:06am

Blank Tests

Test	Status	Time
AIR	Pass	11:07am


Printer Tests

Test	Status	Time
PRNT	Pass	11:07am

CRC Tests

Test	Status	Time
COMP	Pass	11:07am
CAL	Pass	11:07am

Preventive Maintenance
Status: Pass

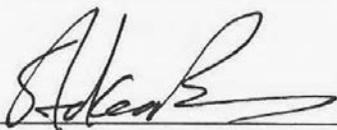

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Vance Instrument Location Vance Co S.O.

Instrument Serial No. 008937 156 Church St Henderson, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

VANCE COUNTY SHERIFF'S DEPARTMENT 900

Serial Number: 008937
Test Date: 08/04/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, STOKES
Permit Number: 11434E
Effective:
04/01/2019-04/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG934303
Exp Date: 12/09/2021


Test	g/210L	Time
DIAG	Pass	10:59am
AIR BLK	.00	11:00am
ACCY CHK	.08	11:01am
AIR BLK	.00	11:02am
SUB TEST	.00	11:02am
AIR BLK	.00	11:03am
SUB TEST	.00	11:05am
AIR BLK	.00	11:05am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

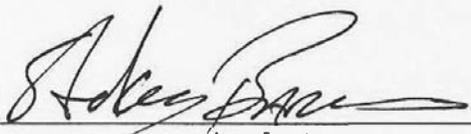

Analyst

Intox EC/IR-II: Preventive Maintenance

VANCE COUNTY SHERIFF'S DEPARTMENT 900

Serial Number: 008937 Test Record Number: 2879
Test Date: 08/04/2020 Test Time: 11:06am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:06am
FLO	Pass	11:06am
FC	Pass	11:06am

Temperature Tests

Test	Status	Time
FC1	Pass	11:06am
SRC	Pass	11:06am
DET	Pass	11:06am
BAR	Pass	11:07am
BT	Pass	11:07am

Blank Tests

Test	Status	Time
AIR	Pass	11:07am

Printer Tests

Test	Status	Time
PRNT	Pass	11:07am

CRC Tests

Test	Status	Time
COMP	Pass	11:07am
CAL	Pass	11:07am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Warren Instrument Location Warren Co LEC
Instrument Serial No. 008793 128 RAFTERS Ln Warrantown, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Stokes Barnes

Signature of Certifying Official

662

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WARREN COUNTY WARREN COUNTY JAIL 920

Serial Number: 008793
Test Date: 08/04/2020

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, STOKES
Permit Number: 11434E
Effective:
04/01/2019-04/01/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG919902
Exp Date: 07/18/2021


Test	g/210L	Time
DIAG	Pass	11:59am
AIR BLK	.00	12:00pm
ACCY CHK	.07	12:01pm
AIR BLK	.00	12:02pm
SUB TEST	.00	12:02pm
AIR BLK	.00	12:03pm
SUB TEST	.00	12:05pm
AIR BLK	.00	12:05pm

Reported AC: 00 g/210L

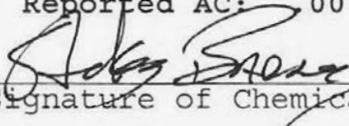

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WARREN COUNTY WARREN COUNTY JAIL 920

Serial Number: 008793 Test Record Number: 1622
Test Date: 08/04/2020 Test Time: 12:06pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:06pm
FLO	Pass	12:06pm
FC	Pass	12:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:06pm
SRC	Pass	12:06pm
DET	Pass	12:06pm
BAR	Pass	12:06pm
BT	Pass	12:06pm

Blank Tests

Test	Status	Time
AIR	Pass	12:07pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:07pm

CRC Tests

Test	Status	Time
COMP	Pass	12:07pm
CAL	Pass	12:07pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wilson Instrument Location Wilson Co. Detention Center
Instrument Serial No. 008627 100 E. Green St., Wilson, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of AUGUST, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



James Kessel
Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILSON COUNTY DETENTION CENTER 970

Serial Number: 008627

Test Date: 08/27/2020

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Keesler, Linda A

Permit Number: 0045-5468

Effective:

07/08/2019-07/08/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG911506

Exp Date: 04/25/2021


Test	g/210L	Time
DIAG	Pass	2:15pm
AIR BLK	.00	2:16pm
ACCY CHK	.08	2:16pm
AIR BLK	.00	2:17pm
SUB TEST	.00	2:18pm
AIR BLK	.00	2:19pm
SUB TEST	.00	2:20pm
AIR BLK	.00	2:21pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WILSON COUNTY DETENTION CENTER 970

Serial Number: 008627 Test Record Number: 2604
Test Date: 08/27/2020 Test Time: 2:23pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:24pm
FLO	Pass	2:24pm
FC	Pass	2:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:24pm
SRC	Pass	2:24pm
DET	Pass	2:24pm
BAR	Pass	2:24pm
BT	Pass	2:24pm

Blank Tests

Test	Status	Time
AIR	Pass	2:25pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:25pm

CRC Tests

Test	Status	Time
COMP	Pass	2:25pm
CAL	Pass	2:25pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wilson Instrument Location Wilson Co. Detention Center
Instrument Serial No. 008652 100 E. Broad St., Wilson, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILSON COUNTY DETENTION CENTER 970

Serial Number: 008652
Test Date: 08/27/2020

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Keesler, Linda A

Permit Number: 0045-5468

Effective:

07/08/2019-07/08/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG919901


Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	2:17pm
AIR BLK	.00	2:18pm
ACCY CHK	.08	2:18pm
AIR BLK	.00	2:19pm
SUB TEST	.00	2:20pm
AIR BLK	.00	2:21pm
SUB TEST	.00	2:22pm
AIR BLK	.00	2:23pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WILSON COUNTY DETENTION CENTER 970

Serial Number: 008652 Test Record Number: 3458
Test Date: 08/27/2020 Test Time: 2:24pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:24pm
FLO	Pass	2:24pm
FC	Pass	2:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:24pm
SRC	Pass	2:24pm
DET	Pass	2:24pm
BAR	Pass	2:24pm
BT	Pass	2:24pm

Blank Tests

Test	Status	Time
AIR	Pass	2:25pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:25pm

CRC Tests

Test	Status	Time
COMP	Pass	2:25pm
CAL	Pass	2:25pm

Preventive Maintenance
Status: Pass



Analyst